

CCD: Mitigating Hallucinations in Radiology MLLMs via Clinical Contrastive Decoding

Xi Zhang [♣], Zaiqiao Meng ^{♣,◇*}, Jake Lever [♣], Edmond S. L. Ho [♣]

[♣]School of Computing Science, University of Glasgow

[◇]Language Technology Lab, University of Cambridge

X.Zhang.6@research.gla.ac.uk, mz468@cam.ac.uk

{Jake.Lever, Shu-Lim.Ho}@glasgow.ac.uk

 <https://x-izhang.github.io/CCD/>

Abstract

Multimodal large language models (MLLMs) have recently achieved remarkable progress in radiology by integrating visual perception with natural language understanding. However, they often generate clinically unsupported descriptions, known as medical hallucinations, which pose serious risks in medical applications that demand accuracy and image-grounded outputs. Through empirical analysis, we find that prompt-induced hallucinations remain prevalent in radiology MLLMs, largely due to oversensitivity to clinical sections. To address this, we introduce Clinical Contrastive Decoding (CCD), a *training-free* and *retrieval-free* inference framework that integrates structured clinical signals from task-specific radiology expert models. CCD introduces a dual-stage contrastive mechanism to refine token-level logits during generation, thereby enhancing clinical fidelity without modifying the base MLLM. Experiments on three datasets and multiple models demonstrate that CCD consistently improves overall performance on radiology report generation (RRG). On the MIMIC-CXR dataset, it yields up to a **17%** improvement in RadGraph-F1 when applied to state-of-the-art RRG models. Our approach provides a lightweight and generalisable solution for mitigating medical hallucinations, effectively bridging expert models and MLLMs in radiology.

1 Introduction

Multimodal large language models (MLLMs) have recently shown substantial promise in the medical domain (AISaad et al., 2024; Shen et al., 2025). By coupling vision encoders with pretrained large language models (LLMs) (Chen et al., 2024a; Liang et al., 2025), MLLMs align visual inputs with language representations (Liu et al., 2024b), enabling complex reasoning and generation across multimodal inputs (Yin et al., 2024; Liu et al., 2024a;

Wang et al., 2024a). Among various medical specialties, radiology has emerged as a key application area (Tu et al., 2025; Saab et al., 2025), where MLLMs are increasingly used to interpret radiographs and articulate diagnostic findings in clinically precise language (Liu et al., 2019). Compared to general-domain settings, radiology imposes significantly stricter demands on factual accuracy and clinical reliability (Chen et al., 2024b).

Despite recent progress, MLLMs remain limited in real-world deployment, primarily due to hallucination (Huang et al., 2025). In clinical contexts, this issue is termed *medical hallucination* (Chen et al., 2024b; Gu et al., 2024), referring to outputs that appear clinically plausible yet unsupported by the medical image or misaligned with diagnostic intent (Zhu et al., 2025). Such errors are particularly consequential in safety-critical fields like radiology, where even minor inaccuracies can adversely affect diagnosis and ultimately compromise patient treatment (Chen et al., 2024b). In these scenarios, generated outputs must be grounded in medical evidence and adhere to established clinical standards (Wu et al., 2024). More related work on radiology MLLMs, medical hallucination, and current mitigation strategies is provided in Appx. A.

Radiology report generation (RRG) involves automatically producing free-text reports from medical images (Liu et al., 2019), such as chest X-rays. As a core task in radiology workflows, it plays a central role in clinical interpretation and is a key benchmark for advancing medical AI (Monshi et al., 2020). Compared to visual question answering (VQA), which addresses narrowly scoped queries, RRG requires holistic image understanding and precise, clinically grounded expression of findings (Yildirim et al., 2024), making it substantially more complex and error-prone. Consequently, medical hallucinations in RRG are often more severe and multi-dimensional, including fabricated pathologies on normal images, misclassification of

* Corresponding author.

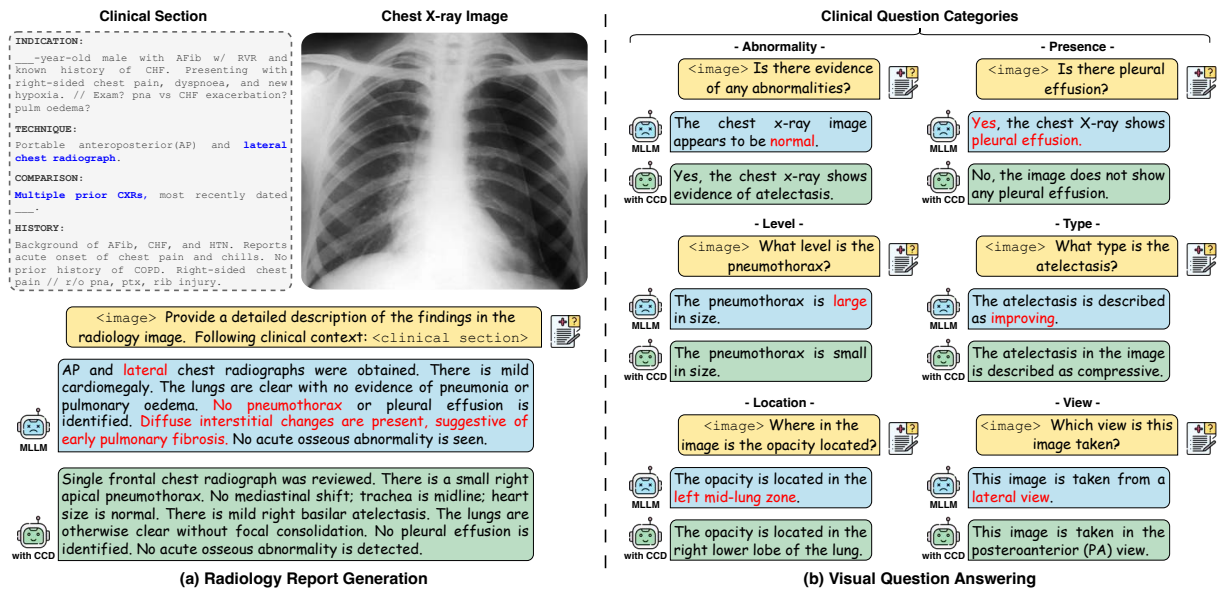


Figure 1: Illustration of medical hallucinations in MLLMs across two tasks: (a) MAIRA-2 (Bannur et al., 2024) for radiology report generation and (b) LLaVA-Med (Li et al., 2023a) for visual question answering. Medical hallucinations are highlighted in red, indicating generated clinical content not supported by the image. Clinically irrelevant or counterfactual information in the reference clinical section is shown in blue. With Clinical Contrastive Decoding (CCD), medical hallucinations in the baseline models are mitigated across both tasks and question types.

finding types or locations, and errors induced by contradictory prompts (Chen et al., 2024b), as in Figure 1 (a). In contrast, hallucinations in VQA typically manifest as isolated factual inconsistencies (Zhu et al., 2025), as in Figure 1 (b).

To mitigate medical hallucinations in RRG, recent work explores strategies including training data restructuring (Zambrano Chaves et al., 2025), clinical section sanitisation with GPT-4V (OpenAI et al., 2024), and applying retrieval-augmented generation (RAG) (Xia et al., 2025; Hou et al., 2025). However, these approaches raise privacy concerns, require costly retraining or proprietary APIs, and remain impractical in low-resource radiology settings where effective retrieval corpora are difficult to construct. To examine medical hallucinations in radiology MLLMs, we conduct an empirical study on RRG in Sec. 2. We find that prompt-induced medical hallucinations (Chen et al., 2024b), caused by clinically implausible or ambiguous prompts, persist despite real-world clinical inputs (Figure 1, top-left). This underscores the need for inference-time solutions beyond dataset-level interventions.

Motivated by the aforementioned observations, we introduce **Clinical Contrastive Decoding (CCD)**, an inference-time method for mitigating medical hallucinations in radiology MLLMs. CCD adopts a two-stage hierarchical contrastive decoding framework that progressively incorporates external clinical signals to guide generation. Specifically, we leverage a task-specific expert model

(e.g., a symptom classifier) to extract structured clinical labels and associated probabilities. Compared to visual representations from the MLLM vision encoder, the expert model captures finer-grained symptom-level information. These signals are integrated in two complementary ways: predicted labels are injected as descriptive prompts to enhance the grounding ability of the MLLM, and probability scores are used to perturb the decoding process, both nudging the outputs toward clinical consistency. This framework enables MLLMs to benefit from additional image-derived knowledge without requiring further alignment or retraining. As a result, **CCD** is a **training-free** and **retrieval-free** approach that operates entirely at inference time to improve radiology MLLMs. This paper makes the following contributions ¹:

❶ We conduct an empirical study on RRG and find that prompt-induced medical hallucinations remain prevalent in radiology MLLMs, often stemming from over-sensitivity to clinical sections.

❷ We propose **CCD**, a general and lightweight inference-time framework that leverages radiology expert models to guide MLLM generation via structured labels and confidence-based guidance.

❸ Extensive experiments across three datasets and multiple models show that **CCD** consistently enhances linguistic quality and clinical fidelity in RRG, while also improving accuracy on VQA.

¹A detailed explanation of our research aims is provided in Appx. B.1, and the study scope is described in Appx. B.2.

Metric	Clinical Section					
	w/o	w/ Indication	w/ Technique	w/ Comparison	w/ History	w/ All
Lexical:						
ROUGE-L	15.60	15.36 ↓0.24	15.61 ↑0.01	12.60 ↓3.00	15.64 ↑0.04	14.83 ↓0.77
BLEU	0.95	1.09 ↑0.14	0.98 ↑0.04	0.81 ↓0.14	1.07 ↑0.12	0.94 ↓0.01
BERTScore	38.19	36.05 ↓2.14	37.41 ↓1.05	30.07 ↓8.12	37.38 ↓0.81	35.53 ↓2.66
Clinical:						
RadGraph-F1	7.59	7.01 ↓0.58	7.35 ↓0.24	5.88 ↓1.71	7.53 ↓0.06	5.80 ↓1.79
Temporal-F1	13.65	12.51 ↓1.14	12.97 ↓0.68	10.13 ↓3.52	13.11 ↓0.54	12.47 ↓1.18
RaTEScore	43.91	43.31 ↓0.61	43.78 ↓0.13	35.10 ↓8.81	43.74 ↓0.17	41.92 ↓1.99
RadEval-BERT	17.53	17.39 ↓0.14	17.07 ↓0.46	13.98 ↓3.57	17.39 ↓0.14	16.48 ↓1.05
<i>CheXbert-F1 (Top5):</i>						
Atelectasis	43.07	37.51 ↓5.56	39.36 ↓3.71	31.29 ↓11.78	38.14 ↓4.93	22.17 ↓20.90
Cardiomegaly	7.49	14.39 ↑6.90	8.01 ↑0.52	6.29 ↓1.20	12.61 ↑5.12	11.45 ↑3.96
Consolidation	2.37	2.36 ↓0.01	2.25 ↓0.12	0.89 ↓1.48	0.78 ↓1.59	9.40 ↑7.03
Edema	11.59	15.11 ↑3.52	0.90 ↓10.69	2.67 ↓8.92	12.48 ↑0.89	19.19 ↑7.60
Pleural Effusion	54.24	48.38 ↓5.86	53.22 ↓1.02	41.84 ↓12.40	52.29 ↓1.95	43.18 ↓11.06

Table 1: **Medical hallucination evaluation on MIMIC-CXR.** The baseline uses greedy decoding without additional clinical section input. “↑” indicates improvement relative to the baseline; “↓” indicates degradation.

2 Medical Hallucination in MLLMs

In this section, we conduct empirical analyses to examine the behaviour of radiology MLLMs. We focus on the chest X-ray modality and the RRG task, which requires comprehensive image understanding and is more susceptible to *prompt-induced medical hallucinations* (Chen et al., 2024b) than VQA. Experiments are conducted on the MIMIC-CXR dataset (Johnson et al., 2019b), which provides clinically detailed reference reports for both hallucination evaluation and generation guidance.

Setup for Medical Hallucinations Prompt-induced hallucinations refer to errors triggered by prompts containing misleading or implausible information, thereby serving as a means to evaluate a model’s robustness in clinically sensitive contexts (Chen et al., 2024b). Previous advanced work has primarily relied on incorporating clinical sections from radiology reports during MLLM training to enhance alignment (Bannur et al., 2024; Zhang et al., 2025c). However, such sections may contain irrelevant or invalid information. For instance, as illustrated in Figure 1 (a) (top-left), the clinical section references a *lateral view* and *prior CXRs*, which are counterfactual given that only a single frontal view is available. To assess such medical hallucinations, we prompt the model with varied clinical sections and evaluate whether it can robustly handle factual inconsistencies while maintaining the quality of the generated report. We choose LLaVA-Med v1.5 (Li et al., 2023a) as our baseline due to its extensive training with radiol-

ogy visual instruction data and strong instruction-following capability. We adopt the default prompt shown in Figure 1 (a) and use greedy decoding, the standard setting for radiology MLLMs. In each case, we append a different clinical section, such as *indication*, *technique*, *comparison*, or *history*, to the end of the default prompt. These sections are extracted using rule-based heuristics from the MIMIC official repository (Johnson et al., 2018).

Evaluation for Report Generation We follow prior work and adopt a set of lexical and radiology-specific metrics (Hyland et al., 2024; Zambrano Chaves et al., 2025), which are widely adopted as standard evaluation protocols in the field. Lexical metrics (ROUGE-L (Lin, 2004), BLEU (Papineni et al., 2002), and BERTScore (Zhang et al., 2020)) assess textual similarity between generated and reference reports. Domain-specific metrics capture clinical correctness, including entity and relation overlap (RadGraph-F1 (Delbrouck et al., 2022)), temporal description accuracy (Temporal-F1 (Zhang et al., 2025c)), concept-level correctness (RaTeScore (Zhao et al., 2024)), semantic consistency (RadEval-BERT (Xu et al., 2025a)), and common finding coverage (CheXbert-F1 (Smit et al., 2020)). Detailed metric definitions and implementation details are provided in Appx. C.2.

Hallucination Drivers: Clinical Context Sensitivity As shown in Table 1, appending different clinical sections leads to varying degrees of performance change. For lexical metrics, sections such

as *history* and *technique* sometimes result in slight score improvements. This may be because these sections contain clinical terminology and standardised phrasing that resemble the narrative style of radiology reports, thereby making the generated text appear more fluent. In contrast, adding the *comparison* section consistently leads to lower scores (e.g., BERTScore $\downarrow 8.12$). This is likely because comparison notes often include references to prior exams or temporal changes, which are not observable in the current frontal image. This mismatch between the textual prompt and the visual input introduces context that the model cannot validate, increasing the likelihood of hallucinated content.

For clinical evaluation metrics, we observe a general decline in report quality across all appended sections. When appending *indication*, there is a modest improvement in detection of certain pathologies, particularly *Cardiomegaly* (CheXbert-F1 $\uparrow 6.90$). This condition often co-occurs with other diseases and is frequently referenced in prior reports or diagnostic histories (Tavora et al., 2012), which may help models retrieve relevant context. Conversely, performance on findings such as *Pleural Effusion* and *Atelectasis* tends to decrease. These are typically late-stage manifestations (Woodring and Reed, 1996) that require fine-grained visual reasoning. When MLLMs place excessive emphasis on clinical textual guidance, they may overlook subtle visual evidence of pathological changes, leading to medical hallucinations. This suggests that such errors partly stem from overreliance on prompt-injected clinical context.

Our empirical observations indicate that clinical sections in original reports are not always reliable sources of guidance for MLLMs during generation. In some cases, they introduce misleading signals that can adversely affect downstream tasks such as RRG. Therefore, selecting clinically relevant and contextually appropriate information is essential, particularly at inference. Motivated by this, our proposed CCD leverages domain-specific image expert models to extract accurate and well-grounded clinical information, avoiding the ambiguity and noise often present in original report sections.

3 Clinical Contrastive Decoding

As discussed in Sec. 2, radiology MLLMs tend to overreact to clinical context, leading to hallucinations that degrade report quality. To address this issue, we propose Clinical Contrastive Decoding (CCD), a practical inference-time framework that dynamically adjusts token logits by incorporating clinically grounded signals from domain-specific expert models. As illustrated in Figure 2, CCD consists of two key stages: (a) Symptom-grounded Contrastive Decoding (SCD), which aligns the MLLM’s self-perception with expert-derived symptom labels to reduce false negatives; and (b) Expert-informed Contrastive Decoding (ECD), which applies expert constraints to suppress false positives. Together, they mitigate both under-detection and over-diagnosis, improving clinical reliability.

Preliminaries of MLLM Generation MLLMs are typically composed of a pretrained visual en-

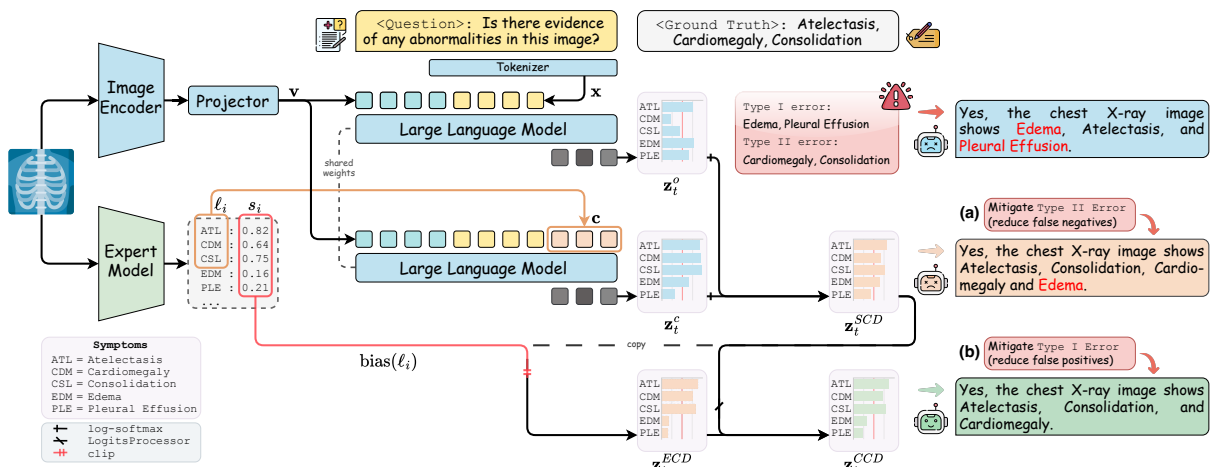


Figure 2: Overview of the CCD framework, which leverages an expert model to enforce clinical consistency in MLLM outputs. During inference, it operates in two stages: (a) **Symptom-grounded Contrastive Decoding**, which incorporates structured clinical labels from the expert model; and (b) **Expert-informed Contrastive Decoding**, which adjusts the latent token logits using expert-derived confidence scores. The output logits are hierarchically calibrated to better match the ground-truth clinical labels. Hallucinated symptoms in the output are marked in red.

coder, a language model as the text decoder, and a projection layer that maps visual tokens into the latent space of the LLM. The projected visual tokens are dimensionally aligned with the embedded text tokens and then fed into the autoregressive language model for generation. For clarity, we denote the projected visual tokens as $\mathbf{v} = \{v_1, v_2, \dots, v_n\}$, where each $v_i \in \mathbb{R}^d$ and d is the hidden dimension. For the default prompt, we represent it as $\mathbf{x} = \{x_1, x_2, \dots, x_m\}$, where each $x_j \in \mathbb{R}^d$ and m is the number of textual tokens. Let f_θ denote the MLLM parameterized by θ . Given the visual tokens \mathbf{v} and textual tokens \mathbf{x} , the model generates a response sequence $\mathbf{y} = \{y_1, \dots, y_T\}$, where each $y_t \in \mathcal{V}$ is a token from the vocabulary of the language model. Accordingly, the output logits at decoding step t are denoted as $\mathbf{z}_t^o = f_\theta(\mathbf{v}, \mathbf{x}, y_{<t}) \in \mathbb{R}^{|\mathcal{V}|}$.

3.1 Symptom-grounded Contrastive Decoding

SCD builds on contrastive decoding (Li et al., 2023b), which encourages generation that aligns with a target model while remaining distinct from a constraint model. This approach balances fluency and factuality by comparing token likelihoods between models. In our setting, we adapt this framework to radiology by introducing symptom-level signals from a task-specific expert model, guiding MLLMs to avoid false negatives without retraining.

Initial Anchor from Experts Given the diverse symptoms encountered in real-world clinical settings, we focus on the 14 common pathology labels defined in the CheXpert ontology (Irvin et al., 2019) as our target set. To obtain symptom-level supervision, we use a DenseNet-based classifier² pre-trained on the MIMIC-CXR dataset (Johnson et al., 2019b) to predict the 14 pathologies from a given \mathbf{v} , which is widely used as a baseline in medical image classification (Baltruschat et al., 2019). From this expert model, we extract a set of clinical labels $\mathcal{L} = \{(\ell_i, s_i)\}_{i=1}^M$, where each ℓ_i denotes a pathology label, and $s_i \in [0, 1]$ represents its predicted probability. These expert-provided symptom labels are filtered using a default threshold (e.g., $s_i > 0.5$), where s_i denotes the calibrated probability output of the expert model after symptom-specific threshold normalisation. Selected labels are then used to construct a concise anchor prompt

²By default, we use the DenseNet from TorchXRaiVision (Cohen et al., 2021) for chest X-ray multi-label prediction. Sec. 4.3 evaluates an alternative expert model, specifically MedSigLIP (Sellergren et al., 2025), via ablation.

(e.g., “Attention to the following clinical instructions: Atelectasis, Cardiomegaly, ...”), denoted as \mathbf{c} , which guides the model during generation.

Self-perception Alignment The model generates its internal symptom representation by producing token-level logits conditioned on the initial clinical anchor. For the same image \mathbf{v} , this can be expressed as $\mathbf{z}_t^c = f_\theta(\mathbf{v}, \mathbf{x} \oplus \mathbf{c}, y_{<t}) \in \mathbb{R}^{|\mathcal{V}|}$, where \oplus denotes concatenation. This design aims to guide the MLLM to generate more relevant symptoms by leveraging the additional clinical context, thereby reducing false negatives. We refer to this guided prediction path as the contrastive branch.

Internal Guidance Following the analysis in Sec. 2, we note that excessive reliance on clinical context can also lead to hallucinations. To balance the influence of the contrastive branch (\mathbf{z}_t^c) and the original decoding branch (\mathbf{z}_t^o), we integrate them using a contrastive decoding mechanism. To ensure numerical stability and facilitate comparison between distributions from different inputs, we convert logits into log-probabilities using log-softmax:

$$\tilde{\mathbf{z}}_t^o = \log \text{softmax}(\mathbf{z}_t^o) \quad (1)$$

$$\tilde{\mathbf{z}}_t^c = \log \text{softmax}(\mathbf{z}_t^c) \quad (2)$$

This transformation mitigates scale and shift sensitivity between outputs, especially when the initial anchor induces large deviations from the original distribution. It also prevents unintended amplification of non-symptom tokens. The generation of the t -th output token is then given by:

$$\mathbf{z}_t^{\text{SCD}} = (1 - \alpha) \tilde{\mathbf{z}}_t^o + \alpha \tilde{\mathbf{z}}_t^c \quad (3)$$

where $\alpha \in [0, 1]$ balances original and anchor-conditioned logits. This encourages the model to align generation with clinically meaningful findings, serving as an internal contrastive signal. At this stage, false negatives are primarily suppressed, as illustrated in Figure 2 (a). Importantly, it remains expert-model-agnostic (see Appx. F.3).

3.2 Expert-informed Contrastive Decoding

Inspired by Bayesian conditional reasoning (Barber, 2012), ECD further incorporates expert model signals to guide the MLLM’s generation process toward clinically plausible outputs.

Probabilistic Guidance For each symptom ℓ_i with probability score s_i , we define a token-level bias using a logit transformation:

$$\text{bias}(\ell_i) = \log \frac{s_i}{1 - s_i} \quad (4)$$

This is necessary because the original probability scores s_i reside in a different space from the MLLM’s token logits \mathbf{z}_t^o , both in scale and semantics, and thus cannot be directly injected into the decoding process. To address this, we convert them into token-aligned logit-based biases, ensuring compatibility with the model’s output distribution and seamless integration during inference.

Diagnostic Plausibility Constraint Inspired by clinical practice, where likelihood ratios of 2, 5, and 10 commonly indicate weak, moderate, and severe diagnostic evidence, respectively (Deeks and Altman, 2004; Grimes and Schulz, 2005), we cap the logit-based bias as follows:

$$\text{bias}(\tilde{\ell}_i) \leftarrow \text{clip}(\text{bias}(\ell_i), -\log(\gamma), +\log(\gamma)) \quad (5)$$

where $\gamma \in \{2, 5, 10\}$. We incorporate the clipped bias to refine the first-stage SCD signal:

$$\mathbf{z}_t^{\text{ECD}} = \mathbf{z}_t^{\text{SCD}} + \text{bias}(\tilde{\ell}_i) \quad (6)$$

where $\tilde{\ell}_i$ is a selected symptom label from the expert model, and its corresponding bias is uniformly added to token logits. This constraint limits over-correction while preserving the generative flexibility of the MLLM. To avoid interfering with inherent decoding behaviour, we apply default decoding controllers on the first-stage SCD logits, as:

$$\tilde{\mathbf{z}}_t^{\text{SCD}} = \text{LogitsProcessor}(\mathbf{z}_t^{\text{SCD}}) \quad (7)$$

where $\text{LogitsProcessor}()$ refers to a stack of standard decoding modules from the Transformers library³ (Wolf et al., 2020). These modules ensure consistent generation behaviour across models.

Sustained Contrastive Adjustment While the first-stage SCD encourages the model to generate more symptom-related content, it may also increase the risk of false positives. To mitigate this, we incorporate expert-informed constraints to suppress clinically unjustified symptoms. Finally, we interpolate between the adjusted SCD logits and the ECD output to produce the final token logits:

$$\mathbf{z}_t^{\text{CCD}} = (1 - \beta) \tilde{\mathbf{z}}_t^{\text{SCD}} + \beta \mathbf{z}_t^{\text{ECD}} \quad (8)$$

where $\beta \in [0, 1]$ balances contributions of internal contrastive and expert-informed logits, preventing over-reliance on true positives while maintaining

³Including commonly used components such as repetition penalties, minimum length constraints, and decoding strategies like temperature scaling, greedy decoding, and beam search.

linguistic fluency. The final next-token distribution is computed as $p(\tilde{y}_t | \cdot) = \text{softmax}(\mathbf{z}_t^{\text{CCD}})$, where \tilde{y}_t denotes the probability of the token generated at decoding step t after dual-stage adjustment.

As illustrated in Figure 2 (b) bottom-right, **CCD** integrates symptom-grounded and expert-informed signals to continuously adjust the MLLM’s output during inference, refining the autoregressive decoding process and mitigating both false negatives and false positives in medical hallucinations.

4 Experiments

In this section, we conduct a series of experiments to evaluate the effectiveness of CCD in mitigating medical hallucinations and improving performance in radiology-specific generation tasks. Our evaluation spans multiple radiology MLLMs, three datasets, and two key tasks: RRG and VQA.

4.1 Experimental Settings

Datasets We evaluate our method on three widely used radiology datasets: the official test splits of MIMIC-CXR (Johnson et al., 2019b) and IU-Xray (Demner-Fushman et al., 2015), and the public validation set of CheXpert Plus (Chambon et al., 2024), as no official test split is available for the latter. Following prior works (Sharma et al., 2025b; Zhang et al., 2025c), we focus on generating the *findings* section from a single frontal-view image for the RRG. For the VQA task, we use Medical-CXR-VQA (Hu et al., 2024), a MIMIC-CXR-derived dataset with six clinical question categories, shown in Figure 1 (b). Details on dataset description and preprocessing are provided in Appx. C.1.

Evaluation Metrics We adopt the same set of metrics described in Sec. 2 to evaluate report generation quality. For the VQA task, we report micro-averaged Recall and F1 based on whether ground-truth labels appear in the generated text. Details on evaluation metrics are provided in Appx. C.2.

Baselines In addition to the default greedy decoding strategy, we compare against several recent training-free hallucination mitigation methods proposed in the general domain, including VCD (Leng et al., 2023), OPERA (Huang et al., 2024), ICD (Wang et al., 2024b), DeCo (Wang et al., 2025a), and Attn-Lens (Jiang et al., 2025b). We evaluate the effectiveness of our proposed CCD on radiology MLLMs, using MAIRA-2 (Bannur et al., 2024), the top open-source model on the ReXRrank leaderboard (Zhang et al., 2024b), as

Method	Lexical Metric			Clinical Metric					
	ROUGE-L	BLEU	BERTScore	RadGraph-F1	Temporal-F1	RaTEScore	RadEval-BERT	CheXbert _{F1} ⁵	CheXbert _{F1} ¹⁴
MIMIC-CXR									
Baseline	19.57	1.61	49.56	16.23	12.11	50.82	16.96	16.14	10.57
+ VCD	19.47	2.02	48.99	15.90	12.57	49.85	17.49	19.17	15.47
+ OPERA	19.18	1.77	49.31	16.06	13.26	50.59	17.09	16.25	11.82
+ ICD	17.43	2.02	46.58	13.65	13.98	47.01	17.13	17.25	12.26
+ DeCO	19.40	1.65	49.33	15.93	12.95	50.65	17.27	16.60	11.57
+ Attn-Lens	19.51	1.68	49.67	16.37	13.45	50.86	17.15	16.74	10.98
+ CCD	20.70	2.10	51.62	19.01	17.58	53.32	17.50	27.05	16.02
△	1.13	0.49	2.06	2.78	5.47	2.50	0.54	10.91	5.45
IU-Xray									
Baseline	18.50	2.67	42.19	16.52	66.06	46.86	20.15	4.02	24.14
+ CCD	20.77	3.31	46.25	21.12	67.16	50.47	22.14	19.96	28.23
△	2.27	0.64	4.06	4.60	1.10	3.61	1.99	15.94	4.09
CheXpert Plus									
Baseline	18.07	1.83	45.91	14.27	22.78	47.47	1.99	13.54	8.39
+ CCD	18.59	1.84	46.64	14.89	32.04	47.55	2.91	14.76	9.75
△	0.52	0.01	0.73	0.62	9.23	0.08	0.92	1.22	1.36

Table 2: **Evaluation on the radiology report generation.** Results on the IU-Xray and CheXpert Plus datasets are reported only for the baseline and our method (CCD). **Best** and second-best results are bolded and underlined, respectively. The Δ row denotes the absolute score improvement over the corresponding baseline.

Model	Question Classification												Overall	
	Abnormality		Presence		View		Location		Level		Type			
	F1	Recall	F1	Recall	F1	Recall	F1	Recall	F1	Recall	F1	Recall	F1	Recall
LLaVA-Med	35.06	21.25	77.72	63.55	39.93	24.95	10.73	5.67	3.84	1.96	10.64	5.62	41.49	26.17
+ CCD	43.16 \uparrow	27.52 \uparrow	80.91 \uparrow	67.94 \uparrow	41.15 \uparrow	26.04 \uparrow	10.23 \downarrow	5.40 \downarrow	3.92 \uparrow	2.06 \uparrow	10.14 \downarrow	5.36 \downarrow	45.11 \uparrow	29.12 \uparrow
CheXagent	61.75	45.74	68.18	59.40	38.28	23.97	7.67	3.99	27.24	15.77	8.54	4.46	47.67	33.12
+ CCD	62.28 \uparrow	45.22 \downarrow	68.83 \uparrow	52.47 \downarrow	39.89 \uparrow	24.91 \uparrow	9.93 \uparrow	5.23 \uparrow	42.50 \uparrow	26.99 \uparrow	8.77 \uparrow	4.59 \uparrow	51.15 \uparrow	34.36 \uparrow

Table 3: **Evaluation on the medical visual question answering.** “ \uparrow ” indicates improvement, “ \downarrow ” denotes degradation relative to the baseline. Appx. G presents a case analysis of two degraded examples from LLaVA-Med.

the baseline for RRG, and medical VQA models, LLaVA-Med (Li et al., 2023a) and CheXagent-8B (Chen et al., 2024c), for VQA. We use the pathology classifier from TorchXRyVision (Cohen et al., 2021) as the expert model to provide symptom-level predictions from chest X-ray images. Additional details on decoding strategies and corresponding results are presented in Appx. E.1.

Implementation Details For all methods, we adopt the default configurations from their original papers to ensure fairness. For CCD, we fix hyperparameters across tasks: in the first stage, the symptom-grounded guidance strength is set to $\alpha = 0.5$; in the second stage, the expert-informed guidance strength is set to $\beta = 0.5$, and the diagnostic plausibility constraint is controlled by $\gamma = 10$. Additional details, including MLLM and expert model settings, are provided in Appx. D.

4.2 Experimental Results

Results on Radiology Report Generation Table 2 shows that CCD improves both lexical and

clinical metrics. Appx. E provides additional comparisons with other methods (Table 5) and reports results across different MLLMs (Table 6). These results indicate that CCD outperforms general-domain decoding strategies, particularly on clinical metrics such as CheXbert_{F1}⁵ ($\uparrow 10.91$) and RadGraph-F1 ($\uparrow 2.78$, $\approx 17\%$ relative improvement) on MIMIC-CXR. Furthermore, it enhances the performance of advanced radiology MLLMs on the RRG task.

Results on Visual Question Answering Table 3 shows that CCD yields improvements across most categories. For LLaVA-Med, a slight drop is observed for *Location* and *Type* questions, mainly due to the broader, morphological nature of these findings (e.g., infiltrates), which are not well captured by the default expert model. Using a stronger backbone, CheXagent-8B, mitigates these modest declines. Nonetheless, CCD maintains competitive overall performance, demonstrating robustness despite the absence of explicit morphological labels.⁴

⁴Additional analyses on the effects of replacing the backbone with CheXagent-8B are provided in Appx. E.3.

Method	Lexical Metric			Clinical Metric					
	ROUGE-L	BLEU	BERTScore	RadGraph-F1	Temporal-F1	RaTEScore	RadEval-BERT	CheXbert _{F1} ⁵	CheXbert _{F1} ¹⁴
CCD	20.70	2.10	51.62	19.01	17.58	53.32	17.50	27.05	16.02
w/o SCD	18.22 ↓	1.26 ↓	49.40 ↓	16.71 ↓	13.81 ↓	51.59 ↓	16.65 ↓	19.02 ↓	12.06 ↓
w/o ECD	20.73 ↑	1.96 ↓	51.72 ↑	18.78 ↓	17.40 ↓	53.21 ↓	17.71 ↑	21.02 ↓	11.47 ↓
w/o All	19.57 ↓	1.61 ↓	49.56 ↓	16.23 ↓	12.11 ↓	50.82 ↓	16.96 ↓	16.14 ↓	10.57 ↓
All-class \mapsto Top-5-class	20.98 ↑	1.95 ↓	51.89 ↑	19.27 ↑	17.99 ↑	53.27 ↓	17.78 ↑	26.78 ↓	14.34 ↓
DenseNet \mapsto MedSigLIP	20.92 ↑	2.24 ↑	51.86 ↑	19.32 ↑	16.80 ↓	53.48 ↑	18.12 ↑	27.42 ↑	16.59 ↑

Table 4: **Ablation studies of CCD.** “w/o” indicates removal of a component; “ \mapsto ” denotes replacement with an alternative expert model setting. “ \uparrow / \downarrow ” indicate performance improvement or degradation relative to the baseline.

4.3 Ablation Studies

As shown in Table 4, we conduct ablation studies on the RRG task using MAIRA-2 to assess the effectiveness of CCD under different configurations, guided by the following research questions.

Are both stages of CCD necessary for performance gains? We evaluate the impact of removing either SCD or ECD. Excluding SCD, which addresses false negatives, leads to a notable decline in CheXbert_{F1}^{5,14}, indicating reduced coverage of symptom-related findings. In contrast, removing ECD causes a relatively smaller drop in clinical metrics compared to SCD, but slightly improves some lexical scores, suggesting its role in suppressing false positives and promoting concise, accurate descriptions. Eliminating both stages results in the most substantial overall degradation, confirming that SCD and ECD are complementary and jointly critical for mitigating medical hallucinations.

Does CCD remain robust under different expert settings? We evaluate the robustness of CCD by varying the expert model configurations, as shown in the last two rows of Table 4. Limiting the expert output to the top-5 most frequent symptoms slightly improves lexical and some clinical metrics, likely because a smaller label space reduces generation complexity. However, it leads to a larger drop in CheXbert_{F1}¹⁴ ($\downarrow 1.68$) compared to CheXbert_{F1}⁵ ($\downarrow 0.27$), underscoring the importance of maintaining broad label space coverage in the pretrained expert model. Replacing the default expert with MedSigLIP (Sellergren et al., 2025), an open-source zero-shot symptom classifier introduced concurrently, yields consistent improvements across both metric types. These results indicate that CCD benefits from stronger expert guidance while remaining robust across expert settings.

What is the effect of guidance strength on generation? We vary the control weights α and β , which modulate the influence of symptom-

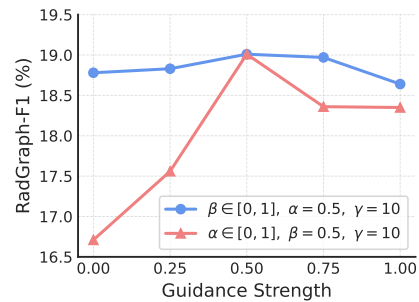


Figure 3: Ablation study of guidance strength (α, β) ranging from 0 to 1, with others fixed at default.

grounded signals and expert-informed confidence scores, respectively. These weights determine how much the expert model guides the radiology MLLM during generation. Figure 3 shows that the model achieves its best empirical RadGraph-F1 score when both guidance strengths reach 0.5, indicating the importance of balanced adjustment.⁵

5 Conclusion

In this work, we address the challenge of prompt-induced hallucinations in radiology MLLMs by introducing **Clinical Contrastive Decoding (CCD)**, a *training-free* and *retrieval-free* inference-time framework. By leveraging a task-specific expert model and dual-stage interventions on the MLLM’s latent logits, CCD further improves clinical consistency in RRG and also contributes to VQA performance, all without retraining or data augmentation. Experiments across diverse models, datasets, and metrics validate its practical effectiveness in radiology tasks. Beyond performance, we highlight the complementary role of foundation expert models in guiding MLLM behaviour, offering a practical path to integrate domain expertise into generation models. As medical AI evolves, we believe CCD represents a modest yet meaningful step toward building more trustworthy and clinically aligned systems that approach physician-level reliability.

⁵Ablation studies are provided in Appx. F.1, which includes tables and the ablation study of the plausibility constraint (γ); Appx. F.2 reports results from random tests; Appx. F.3 provides analyses on additional expert label types.

Limitations

Despite the effectiveness of our approach in mitigating medical hallucinations in radiology MLLMs, several limitations remain. For example, our experiments are conducted on standard benchmark datasets, which may not fully reflect the diversity of image acquisition conditions encountered in real-world clinical practice. The applicability of CCD to data from non-standard or heterogeneous imaging setups therefore warrants further investigation.

Although clinical deployment requires highly reliable outputs, our evaluation relies on automatic metrics and does not include human expert assessment. We recognise that evaluation by radiologists would offer a more comprehensive and clinically grounded validation of model behaviour, particularly in safety-critical scenarios. However, such studies are prohibitively expensive and resource-intensive, and are beyond the scope of this work. A more detailed discussion is provided in Appx. H.

Ethical Considerations

This study is conducted entirely using publicly available and de-identified datasets. We adhere to the ethical guidelines and usage policies of each dataset, complying with standards equivalent to exempt human subjects research. By relying on open-access data, we promote transparency, reproducibility, and ethical integrity. All chest X-ray images shown in figures are blurred to preserve privacy and minimise visual discomfort.

Our work aims to support medical AI systems as assistive tools for licensed clinicians rather than replacements. Although such systems can improve clinical efficiency, they must be deployed responsibly with appropriate clinical oversight. To mitigate risks associated with over-reliance on automated outputs, we encourage the inclusion of human expert evaluation and human-in-the-loop validation in future deployment. We advocate for a collaborative integration of AI and medical expertise to ensure safe and equitable clinical use.

References

Rawan AlSaad, Alaa Abd-Alrazaq, Sabri Boughorbel, Arfan Ahmed, Max-Antoine Renault, Rafat Damseh, and Javaid Sheikh. 2024. [Multimodal large language models in health care: applications, challenges, and future outlook](#). *Journal of medical Internet research*, 26:e59505.

Wenbin An, Feng Tian, Sicong Leng, Jiahao Nie, Haonan Lin, QianYing Wang, Ping Chen, Xiaoqin Zhang, and Shijian Lu. 2025. [Mitigating object hallucinations in large vision-language models with assembly of global and local attention](#). *Preprint*, arXiv:2406.12718.

Ivo M Baltruschat, Hannes Nickisch, Michael Grass, Tobias Knopp, and Axel Saalbach. 2019. [Comparison of deep learning approaches for multi-label chest x-ray classification](#). *Scientific reports*, 9(1):6381.

Oishi Banerjee, Hong-Yu Zhou, Subathra Adithan, Stephen Kwak, Kay Wu, and Pranav Rajpurkar. 2024. [Direct preference optimization for suppressing hallucinated prior exams in radiology report generation](#). *Preprint*, arXiv:2406.06496.

Shruthi Bannur, Kenza Bouzid, Daniel C. Castro, Anton Schwaighofer, Anja Thieme, Sam Bond-Taylor, Maximilian Ilse, Fernando Pérez-García, Valentina Salvatelli, Harshita Sharma, Felix Meissen, Mercy Ranjit, Shaury Srivastav, Julia Gong, Noel C. F. Codella, Fabian Falck, Ozan Oktay, Matthew P. Lungren, Maria Teodora Wetscherek, and 2 others. 2024. [Maira-2: Grounded radiology report generation](#). *Preprint*, arXiv:2406.04449.

D. Barber. 2012. [Bayesian Reasoning and Machine Learning](#). Bayesian Reasoning and Machine Learning. Cambridge University Press.

Pierre Chambon, Jean-Benoit Delbrouck, Thomas Sounack, Shih-Cheng Huang, Zhihong Chen, Maya Varma, Steven QH Truong, Chu The Chuong, and Curtis P. Langlotz. 2024. [Chexpert plus: Augmenting a large chest x-ray dataset with text radiology reports, patient demographics and additional image formats](#). *Preprint*, arXiv:2405.19538.

Boyuan Chen, Zhuo Xu, Sean Kirmani, Brian Ichter, Danny Driess, Pete Florence, Dorsa Sadigh, Leonidas Guibas, and Fei Xia. 2024a. [Spatialvlm: Endowing vision-language models with spatial reasoning capabilities](#). *Preprint*, arXiv:2401.12168.

Jiawei Chen, Dingkan Yang, Tong Wu, Yue Jiang, Xiaolu Hou, Mingcheng Li, Shunli Wang, Dongling Xiao, Ke Li, and Lihua Zhang. 2024b. [Detecting and evaluating medical hallucinations in large vision language models](#). *Preprint*, arXiv:2406.10185.

Zeming Chen, Alejandro Hernández-Cano, Angelika Romanou, Antoine Bonnet, Kyle Matoba, Francesco Salvi, Matteo Pagliardini, Simin Fan, Andreas Köpf, Amirkeivan Mohtashami, Alexandre Sallinen, Alireza Sakhaeirad, Vinitra Swamy, Igor Krawczuk, Deniz Bayazit, Axel Marmet, Syrielle Montariol, Mary-Anne Hartley, Martin Jaggi, and Antoine Bosselut. 2023. [Meditron-70b: Scaling medical pretraining for large language models](#). *Preprint*, arXiv:2311.16079.

Zhihong Chen, Maya Varma, Jean-Benoit Delbrouck, Magdalini Paschali, Louis Blankemeier, Dave Van Veen, Jeya Maria Jose Valanarasu, Alaa Youssef,

- Joseph Paul Cohen, Eduardo Pontes Reis, Emily B. Tsai, Andrew Johnston, Cameron Olsen, Tanishq Mathew Abraham, Sergios Gatidis, Akshay S Chaudhari, and Curtis Langlotz. 2024c. [Chexagent: Towards a foundation model for chest x-ray interpretation](#). *arXiv preprint arXiv:2401.12208*.
- Wei-Lin Chiang, Zhuohan Li, Zi Lin, Ying Sheng, Zhanghao Wu, Hao Zhang, Lianmin Zheng, Siyuan Zhuang, Yonghao Zhuang, Joseph E. Gonzalez, Ion Stoica, and Eric P. Xing. 2023. [Vicuna: An open-source chatbot impressing gpt-4 with 90%* chatgpt quality](#).
- Joseph Paul Cohen, Joseph D. Viviano, Paul Bertin, Paul Morrison, Parsa Torabian, Matteo Guarrera, Matthew P Lungren, Akshay Chaudhari, Rupert Brooks, Mohammad Hashir, and Hadrien Bertrand. 2021. [Torchxrayvision: A library of chest x-ray datasets and models](#). *Preprint*, arXiv:2111.00595.
- Jonathan J Deeks and Douglas G Altman. 2004. [Diagnostic tests 4: likelihood ratios](#). *Bmj*, 329(7458):168–169.
- Jean-Benoit Delbrouck, Pierre Chambon, Christian Bluethgen, Emily Tsai, Omar Almusa, and Curtis Langlotz. 2022. [Improving the factual correctness of radiology report generation with semantic rewards](#). In *Findings of the Association for Computational Linguistics: EMNLP 2022*, pages 4348–4360, Abu Dhabi, United Arab Emirates. Association for Computational Linguistics.
- Dina Demner-Fushman, Marc D Kohli, Marc B Rosenman, Sonya E Shooshan, Laritza Rodriguez, Sameer Antani, George R Thoma, and Clement J McDonald. 2015. [Preparing a collection of radiology examinations for distribution and retrieval](#). *Journal of the American Medical Informatics Association*, 23(2):304–310.
- Jacob Devlin, Ming-Wei Chang, Kenton Lee, and Kristina Toutanova. 2019. [Bert: Pre-training of deep bidirectional transformers for language understanding](#). *Preprint*, arXiv:1810.04805.
- Alessandro Favero, Luca Zancato, Matthew Trager, Siddharth Choudhary, Pramuditha Perera, Alessandro Achille, Ashwin Swaminathan, and Stefano Soatto. 2024. [Multi-modal hallucination control by visual information grounding](#). *Preprint*, arXiv:2403.14003.
- Sreyan Ghosh, Chandra Kiran Reddy Evuru, Sonal Kumar, Utkarsh Tyagi, Oriol Nieto, Zeyu Jin, and Dinesh Manocha. 2025. [Visual description grounding reduces hallucinations and boosts reasoning in lvlms](#). *Preprint*, arXiv:2405.15683.
- David A Grimes and Kenneth F Schulz. 2005. [Refining clinical diagnosis with likelihood ratios](#). *The Lancet*, 365(9469):1500–1505.
- Zishan Gu, Changchang Yin, Fenglin Liu, and Ping Zhang. 2024. [Medvh: Towards systematic evaluation of hallucination for large vision language models in the medical context](#). *Preprint*, arXiv:2407.02730.
- Paul Hager, Friederike Jungmann, Robbie Holland, Kunal Bhagat, Inga Hubrecht, Manuel Knauer, Jakob Vielhauer, Marcus Makowski, Rickmer Braren, Georgios Kaissis, and 1 others. 2024. [Evaluation and mitigation of the limitations of large language models in clinical decision-making](#). *Nature medicine*, 30(9):2613–2622.
- Wenjun Hou, Yi Cheng, Kaishuai Xu, Heng Li, Yan Hu, Wenjie Li, and Jiang Liu. 2025. [Radar: Enhancing radiology report generation with supplementary knowledge injection](#). *Preprint*, arXiv:2505.14318.
- Edward J. Hu, Yelong Shen, Phillip Wallis, Zeyuan Allen-Zhu, Yuanzhi Li, Shean Wang, Lu Wang, and Weizhu Chen. 2021. [Lora: Low-rank adaptation of large language models](#). *Preprint*, arXiv:2106.09685.
- Xinyue Hu, Lin Gu, Kazuma Kobayashi, Liangchen Liu, Mengliang Zhang, Tatsuya Harada, Ronald M Summers, and Yingying Zhu. 2024. [Interpretable medical image visual question answering via multi-modal relationship graph learning](#). *Medical Image Analysis*, 97:103279.
- Jonathan Huang, Luke Neill, Matthew Wittbrodt, David Melnick, Matthew Klug, Michael Thompson, John Bailitz, Timothy Loftus, Sanjeev Malik, Amit Phull, and 1 others. 2023. [Generative artificial intelligence for chest radiograph interpretation in the emergency department](#). *JAMA network open*, 6(10):e2336100–e2336100.
- Lei Huang, Weijiang Yu, Weitao Ma, Weihong Zhong, Zhangyin Feng, Haotian Wang, Qianglong Chen, Weihua Peng, Xiaocheng Feng, Bing Qin, and 1 others. 2025. [A survey on hallucination in large language models: Principles, taxonomy, challenges, and open questions](#). *ACM Transactions on Information Systems*, 43(2):1–55.
- Qidong Huang, Xiaoyi Dong, Pan Zhang, Bin Wang, Conghui He, Jiaqi Wang, Dahua Lin, Weiming Zhang, and Nenghai Yu. 2024. [Opera: Alleviating hallucination in multi-modal large language models via over-trust penalty and retrospection-allocation](#). *Preprint*, arXiv:2311.17911.
- Stephanie L. Hyland, Shruthi Bannur, Kenza Bouzid, Daniel C. Castro, Mercy Ranjit, Anton Schwaighofer, Fernando Pérez-García, Valentina Salvatelli, Shaury Srivastav, Anja Thieme, Noel Codella, Matthew P. Lungren, Maria Teodora Wetscherek, Ozan Oktay, and Javier Alvarez-Valle. 2024. [Maira-1: A specialised large multimodal model for radiology report generation](#). *Preprint*, arXiv:2311.13668.
- Jeremy Irvin, Pranav Rajpurkar, Michael Ko, Yifan Yu, Silvana Ciurea-Ilcus, Chris Chute, Henrik Marklund, Behzad Haghgoo, Robyn Ball, Katie Shpanskaya, Jayne Seekins, David A. Mong, Safwan S. Halabi, Jesse K. Sandberg, Ricky Jones, David B. Larson, Curtis P. Langlotz, Bhavik N. Patel, Matthew P. Lungren, and Andrew Y. Ng. 2019. [Chexpert: A large chest radiograph dataset with uncertainty labels and expert comparison](#). *Preprint*, arXiv:1901.07031.

- Albert Q. Jiang, Alexandre Sablayrolles, Arthur Mensch, Chris Bamford, Devendra Singh Chaplot, Diego de las Casas, Florian Bressand, Gianna Lengyel, Guillaume Lample, Lucile Saulnier, L  lio Renard Lavaud, Marie-Anne Lachaux, Pierre Stock, Teven Le Scao, Thibaut Lavril, Thomas Wang, Timoth  e Lacroix, and William El Sayed. 2023. [Mistral 7b](#). *Preprint*, arXiv:2310.06825.
- Yue Jiang, Jiawei Chen, Ding kang Yang, Mingcheng Li, Shunli Wang, Tong Wu, Ke Li, and Lihua Zhang. 2025a. [Comt: Chain-of-medical-thought reduces hallucination in medical report generation](#). *Preprint*, arXiv:2406.11451.
- Zhangqi Jiang, Junkai Chen, Beier Zhu, Tingjin Luo, Yankun Shen, and Xu Yang. 2025b. [Devils in middle layers of large vision-language models: Interpreting, detecting and mitigating object hallucinations via attention lens](#). *Preprint*, arXiv:2411.16724.
- Alistair E. W. Johnson, Tom J. Pollard, Nathaniel R. Greenbaum, Matthew P. Lungren, Chih ying Deng, Yifan Peng, Zhiyong Lu, Roger G. Mark, Seth J. Berkowitz, and Steven Horng. 2019a. [Mimic-cxr-jpg, a large publicly available database of labeled chest radiographs](#). *Preprint*, arXiv:1901.07042.
- Alistair EW Johnson, Tom J Pollard, Seth J Berkowitz, Nathaniel R Greenbaum, Matthew P Lungren, Chihying Deng, Roger G Mark, and Steven Horng. 2019b. [Mimic-cxr, a de-identified publicly available database of chest radiographs with free-text reports](#). *Scientific data*, 6(1):317.
- Alistair EW Johnson, David J Stone, Leo A Celi, and Tom J Pollard. 2018. [The mimic code repository: enabling reproducibility in critical care research](#). *Journal of the American Medical Informatics Association*, 25(1):32–39.
- Yubin Kim, Hyewon Jeong, Shan Chen, Shuyue Stella Li, Chanwoo Park, Mingyu Lu, Kumail Alhamoud, Jimin Mun, Cristina Grau, Minseok Jung, Rodrigo Gameiro, Lizhou Fan, Eugene Park, Tristan Lin, Joonsik Yoon, Wonjin Yoon, Maarten Sap, Yulia Tsvetkov, Paul Liang, and 8 others. 2025. [Medical hallucinations in foundation models and their impact on healthcare](#). *Preprint*, arXiv:2503.05777.
- Yuxiang Lai, Jike Zhong, Ming Li, Shitian Zhao, and Xiaofeng Yang. 2025. [Med-rl: Reinforcement learning for generalizable medical reasoning in vision-language models](#). *Preprint*, arXiv:2503.13939.
- Sicong Leng, Hang Zhang, Guanzheng Chen, Xin Li, Shijian Lu, Chunyan Miao, and Lidong Bing. 2023. [Mitigating object hallucinations in large vision-language models through visual contrastive decoding](#). *Preprint*, arXiv:2311.16922.
- Binxu Li, Tiankai Yan, Yuanting Pan, Jie Luo, Ruiyang Ji, Jiayuan Ding, Zhe Xu, Shilong Liu, Haoyu Dong, Zihao Lin, and Yixin Wang. 2024. [Mmedagent: Learning to use medical tools with multi-modal agent](#). *Preprint*, arXiv:2407.02483.
- Chunyuan Li, Cliff Wong, Sheng Zhang, Naoto Usuyama, Haotian Liu, Jianwei Yang, Tristan Naumann, Hoifung Poon, and Jianfeng Gao. 2023a. [LLaVA-med: Training a large language-and-vision assistant for biomedicine in one day](#). In *Thirty-seventh Conference on Neural Information Processing Systems Datasets and Benchmarks Track*.
- Geng Li, Jinglin Xu, Yunzhen Zhao, and Yuxin Peng. 2025a. [Dyfo: A training-free dynamic focus visual search for enhancing lmms in fine-grained visual understanding](#). *Preprint*, arXiv:2504.14920.
- Xiang Lisa Li, Ari Holtzman, Daniel Fried, Percy Liang, Jason Eisner, Tatsunori Hashimoto, Luke Zettlemoyer, and Mike Lewis. 2023b. [Contrastive decoding: Open-ended text generation as optimization](#). *Preprint*, arXiv:2210.15097.
- Zhuowei Li, Haizhou Shi, Yunhe Gao, Di Liu, Zhen-ting Wang, Yuxiao Chen, Ting Liu, Long Zhao, Hao Wang, and Dimitris N. Metaxas. 2025b. [The hidden life of tokens: Reducing hallucination of large vision-language models via visual information steering](#). *Preprint*, arXiv:2502.03628.
- Chia Xin Liang, Pu Tian, Caitlyn Heqi Yin, Yao Yua, Wei An-Hou, Li Ming, Xinyuan Song, Tianyang Wang, Ziqian Bi, and Ming Liu. 2025. [A comprehensive survey and guide to multimodal large language models in vision-language tasks](#). *Preprint*, arXiv:2411.06284.
- Chin-Yew Lin. 2004. [ROUGE: A package for automatic evaluation of summaries](#). In *Text Summarization Branches Out*, pages 74–81, Barcelona, Spain. Association for Computational Linguistics.
- Guanxiong Liu, Tzu-Ming Harry Hsu, Matthew McDermott, Willie Boag, Wei-Hung Weng, Peter Szolovits, and Marzyeh Ghassemi. 2019. [Clinically accurate chest x-ray report generation](#). *Preprint*, arXiv:1904.02633.
- Hanchao Liu, Wenyan Xue, Yifei Chen, Dapeng Chen, Xiutian Zhao, Ke Wang, Liping Hou, Rongjun Li, and Wei Peng. 2024a. [A survey on hallucination in large vision-language models](#). *Preprint*, arXiv:2402.00253.
- Haotian Liu, Chunyuan Li, Yuheng Li, and Yong Jae Lee. 2024b. [Improved baselines with visual instruction tuning](#). *Preprint*, arXiv:2310.03744.
- Haotian Liu, Chunyuan Li, Qingyang Wu, and Yong Jae Lee. 2023. [Visual instruction tuning](#). *Preprint*, arXiv:2304.08485.
- Jiaxiang Liu, Yuan Wang, Jiawei Du, Joey Tianyi Zhou, and Zuo Zhu Liu. 2024c. [Medcot: Medical chain of thought via hierarchical expert](#). *Preprint*, arXiv:2412.13736.
- Sheng Liu, Haotian Ye, Lei Xing, and James Zou. 2024d. [Reducing hallucinations in vision-language models via latent space steering](#). *Preprint*, arXiv:2410.15778.

- Shi Liu, Kecheng Zheng, and Wei Chen. 2024e. [Paying more attention to image: A training-free method for alleviating hallucination in llms](#). *Preprint*, arXiv:2407.21771.
- Kyungmin Min, Minbeom Kim, Kang il Lee, Dongryeol Lee, and Kyomin Jung. 2025. [Mitigating hallucinations in large vision-language models via summary-guided decoding](#). *Preprint*, arXiv:2410.13321.
- Maram Mahmoud A Monshi, Josiah Poon, and Vera Chung. 2020. [Deep learning in generating radiology reports: A survey](#). *Artificial Intelligence in Medicine*, 106:101878.
- OpenAI, Josh Achiam, Steven Adler, Sandhini Agarwal, Lama Ahmad, Ilge Akkaya, Florencia Leoni Aleman, Diogo Almeida, Janko Altmenschmidt, Sam Altman, Shyamal Anadkat, Red Avila, Igor Babuschkin, Suchir Balaji, Valerie Balcom, Paul Baltescu, Haiming Bao, Mohammad Bavarian, Jeff Belgum, and 262 others. 2024. [Gpt-4 technical report](#). *Preprint*, arXiv:2303.08774.
- Sophie Ostmeier, Justin Xu, Zhihong Chen, Maya Varma, Louis Blankemeier, Christian Bluethgen, Arne Edward Michalson Md, Michael Moseley, Curtis Langlotz, Akshay S Chaudhari, and Jean-Benoit Delbrouck. 2024. [Green: Generative radiology report evaluation and error notation](#). In *Findings of the Association for Computational Linguistics: EMNLP 2024*, page 374–390. Association for Computational Linguistics.
- Kishore Papineni, Salim Roukos, Todd Ward, and Wei-Jing Zhu. 2002. [Bleu: a method for automatic evaluation of machine translation](#). In *Proceedings of the 40th Annual Meeting on Association for Computational Linguistics*, ACL '02, page 311–318, USA. Association for Computational Linguistics.
- Fernando Pérez-García, Harshita Sharma, Sam Bond-Taylor, Kenza Bouzid, Valentina Salvatelli, Maximilian Ilse, Shruthi Bannur, Daniel C. Castro, Anton Schwaighofer, Matthew P. Lungren, Maria Wetscherek, Noel Codella, Stephanie L. Hyland, Javier Alvarez-Valle, and Ozan Oktay. 2024. [RAD-DINO: Exploring scalable medical image encoders beyond text supervision](#). *Preprint*, arXiv:2401.10815.
- Fernando Pérez-García, Harshita Sharma, Sam Bond-Taylor, Kenza Bouzid, Valentina Salvatelli, Maximilian Ilse, Shruthi Bannur, Daniel C. Castro, Anton Schwaighofer, Matthew P. Lungren, Maria Teodora Wetscherek, Noel Codella, Stephanie L. Hyland, Javier Alvarez-Valle, and Ozan Oktay. 2025. [Exploring scalable medical image encoders beyond text supervision](#). *Nature Machine Intelligence*, 7(1):119–130.
- Alec Radford, Jong Wook Kim, Chris Hallacy, Aditya Ramesh, Gabriel Goh, Sandhini Agarwal, Girish Sastry, Amanda Askell, Pamela Mishkin, Jack Clark, Gretchen Krueger, and Ilya Sutskever. 2021. [Learning transferable visual models from natural language supervision](#). *Preprint*, arXiv:2103.00020.
- Mercy Ranjit and Tanuja Ganu. 2025. [Rad-phi4-vision-cxr: A compact multimodal assistant for versatile radiology workflows](#). In *Machine Learning for Health Symposium 2025*. Microsoft, Proceedings of Machine Learning Research (PMLR).
- Carveth Read. 1910. [Logic, Deductive and Inductive](#). A. Moring.
- Khaled Saab, Jan Freyberg, Chunjong Park, Tim Strother, Yong Cheng, Wei-Hung Weng, David G. T. Barrett, David Stutz, Nenad Tomasev, Anil Palepu, Valentin Liévin, Yash Sharma, Roma Ruparel, Abdullah Ahmed, Elahe Vedadi, Kimberly Kanada, Cian Hughes, Yun Liu, Geoff Brown, and 17 others. 2025. [Advancing conversational diagnostic ai with multimodal reasoning](#). *Preprint*, arXiv:2505.04653.
- Pranab Sahoo, Prabhash Meharia, Akash Ghosh, Sriparna Saha, Vinija Jain, and Aman Chadha. 2024. [A comprehensive survey of hallucination in large language, image, video and audio foundation models](#). *Preprint*, arXiv:2405.09589.
- Andrew Sellergren, Sahar Kazemzadeh, Tiam Jaroensri, Atila Kiraly, Madeleine Traverse, Timo Kohlberger, Shawn Xu, Fayaz Jamil, Cian Hughes, Charles Lau, Justin Chen, Fereshteh Mahvar, Liron Yatziv, Tiffany Chen, Bram Sterling, Stefanie Anna Baby, Susanna Maria Baby, Jeremy Lai, Samuel Schmidgall, and 62 others. 2025. [Medgemma technical report](#). *Preprint*, arXiv:2507.05201.
- Harshita Sharma, Maxwell C. Reynolds, Valentina Salvatelli, Anne-Marie G. Sykes, Kelly K. Horst, Anton Schwaighofer, Maximilian Ilse, Olesya Melnichenko, Sam Bond-Taylor, Fernando Pérez-García, Vamshi K. Mugu, Alex Chan, Ceylan Colak, Shelby A. Swartz, Motassem B. Nashawaty, Austin J. Gonzalez, Heather A. Ouellette, Selnur B. Erdal, Beth A. Schueler, and 10 others. 2025a. [Closing the performance gap between ai and radiologists in chest x-ray reporting](#). *Preprint*, arXiv:2511.21735.
- Harshita Sharma, Valentina Salvatelli, Shaury Srivastav, Kenza Bouzid, Shruthi Bannur, Daniel C. Castro, Maximilian Ilse, Sam Bond-Taylor, Mercy Prasanna Ranjit, Fabian Falck, Fernando Pérez-García, Anton Schwaighofer, Hannah Richardson, Maria Wetscherek, Stephanie Hyland, and Javier Alvarez-Valle. 2025b. [Maira-seg: Enhancing radiology report generation with segmentation-aware multimodal large language models](#). In *Proceedings of the 4th Machine Learning for Health Symposium*, volume 259 of *Proceedings of Machine Learning Research*, pages 941–960. PMLR.
- Yiqiu Shen, Yanqi Xu, Jiajian Ma, Wushuang Rui, Chen Zhao, Laura Heacock, and Chenchan Huang. 2025. [Multi-modal large language models in radiology: principles, applications, and potential](#). *Abdominal Radiology*, 50(6):2745–2757.

- Peeyush Singhal, Rahee Walambe, Sheela Ramanna, and Ketan Kotecha. 2023. [Domain adaptation: challenges, methods, datasets, and applications](#). *IEEE access*, 11:6973–7020.
- Akshay Smit, Saahil Jain, Pranav Rajpurkar, Anuj Pareek, Andrew Y. Ng, and Matthew P. Lungren. 2020. [Chexbert: Combining automatic labelers and expert annotations for accurate radiology report labeling using bert](#). *Preprint*, arXiv:2004.09167.
- Liwen Sun, James Zhao, Megan Han, and Chenyan Xiong. 2025. [Fact-aware multimodal retrieval augmentation for accurate medical radiology report generation](#). *Preprint*, arXiv:2407.15268.
- Feilong Tang, Chengzhi Liu, Zhongxing Xu, Ming Hu, Zelin Peng, Zhiwei Yang, Jionglong Su, Minquan Lin, Yifan Peng, Xuilian Cheng, Imran Razzak, and Zongyuan Ge. 2025. [Seeing far and clearly: Mitigating hallucinations in mllms with attention causal decoding](#). *Preprint*, arXiv:2505.16652.
- Fabio Tavora, Y Zhang, M Zhang, L Li, M Ripple, D Fowler, and Allen Burke. 2012. [Cardiomegaly is a common arrhythmogenic substrate in adult sudden cardiac deaths, and is associated with obesity](#). *Pathology-Journal of the RCPA*, 44(3):187–191.
- LASA Team, Weiwen Xu, Hou Pong Chan, Long Li, Mahani Aljunied, Ruifeng Yuan, Jianyu Wang, Chenghao Xiao, Guizhen Chen, Chaoqun Liu, Zhaodonghui Li, Yu Sun, Junao Shen, Chaojun Wang, Jie Tan, Deli Zhao, Tingyang Xu, Hao Zhang, and Yu Rong. 2025. [Lingshu: A generalist foundation model for unified multimodal medical understanding and reasoning](#). *Preprint*, arXiv:2506.07044.
- S. M Towhidul Islam Tonmoy, S M Mehedi Zaman, Vinija Jain, Anku Rani, Vipula Rawte, Aman Chadha, and Amitava Das. 2024. [A comprehensive survey of hallucination mitigation techniques in large language models](#). *Preprint*, arXiv:2401.01313.
- Tao Tu, Shekoofeh Azizi, Danny Driess, Mike Schaeckermann, Mohamed Amin, Pi-Chuan Chang, Andrew Carroll, Chuck Lau, Ryutaro Tanno, Ira Ktena, Basil Mustafa, Aakanksha Chowdhery, Yun Liu, Simon Kornblith, David Fleet, Philip Mansfield, Sushant Prakash, Renee Wong, Sunny Virmani, and 13 others. 2023. [Towards generalist biomedical ai](#). *Preprint*, arXiv:2307.14334.
- Tao Tu, Mike Schaeckermann, Anil Palepu, Khaled Saab, Jan Freyberg, Ryutaro Tanno, Amy Wang, Brenna Li, Mohamed Amin, Yong Cheng, and 1 others. 2025. [Towards conversational diagnostic artificial intelligence](#). *Nature*, pages 1–9.
- Chenxi Wang, Xiang Chen, Ningyu Zhang, Bozhong Tian, Haoming Xu, Shumin Deng, and Huajun Chen. 2025a. [Mllm can see? dynamic correction decoding for hallucination mitigation](#). *Preprint*, arXiv:2410.11779.
- Jiaqi Wang, Hanqi Jiang, Yiheng Liu, Chong Ma, Xu Zhang, Yi Pan, Mengyuan Liu, Peiran Gu, Sichen Xia, Wenjun Li, Yutong Zhang, Zihao Wu, Zhengliang Liu, Tianyang Zhong, Bao Ge, Tuo Zhang, Ning Qiang, Xintao Hu, Xi Jiang, and 5 others. 2024a. [A comprehensive review of multimodal large language models: Performance and challenges across different tasks](#). *Preprint*, arXiv:2408.01319.
- Wenxuan Wang, Zizhan Ma, Zheng Wang, Chenghan Wu, Jiaming Ji, Wenting Chen, Xiang Li, and Yixuan Yuan. 2025b. [A survey of llm-based agents in medicine: How far are we from baymax?](#) *Preprint*, arXiv:2502.11211.
- Xiaosong Wang, Yifan Peng, Le Lu, Zhiyong Lu, and Ronald M. Summers. 2018. [Tienet: Text-image embedding network for common thorax disease classification and reporting in chest x-rays](#). *Preprint*, arXiv:1801.04334.
- Xintong Wang, Jingheng Pan, Liang Ding, and Chris Biemann. 2024b. [Mitigating hallucinations in large vision-language models with instruction contrastive decoding](#). *Preprint*, arXiv:2403.18715.
- Benjamin Warner, Antoine Chaffin, Benjamin Clavié, Orion Weller, Oskar Hallström, Said Taghadouini, Alexis Gallagher, Raja Biswas, Faisal Ladhak, Tom Aarsen, Nathan Cooper, Griffin Adams, Jeremy Howard, and Iacopo Poli. 2024. [Smarter, better, faster, longer: A modern bidirectional encoder for fast, memory efficient, and long context finetuning and inference](#). *Preprint*, arXiv:2412.13663.
- Thomas Wolf, Lysandre Debut, Victor Sanh, Julien Chaumond, Clement Delangue, Anthony Moi, Pierric Cistac, Tim Rault, Rémi Louf, Morgan Funtowicz, Joe Davison, Sam Shleifer, Patrick von Platen, Clara Ma, Yacine Jernite, Julien Plu, Canwen Xu, Teven Le Scao, Sylvain Gugger, and 3 others. 2020. [Transformers: State-of-the-art natural language processing](#). In *Proceedings of the 2020 Conference on Empirical Methods in Natural Language Processing: System Demonstrations*, pages 38–45, Online. Association for Computational Linguistics.
- Sangmin Woo, Donguk Kim, Jaehyuk Jang, Yubin Choi, and Changick Kim. 2025. [Don't miss the forest for the trees: Attentional vision calibration for large vision language models](#). *Preprint*, arXiv:2405.17820.
- John H Woodring and James C Reed. 1996. [Types and mechanisms of pulmonary atelectasis](#). *Journal of thoracic imaging*, 11(2):92–108.
- Chaoyi Wu, Jiayu Lei, Qiaoyu Zheng, Weike Zhao, Weixiong Lin, Xiaoman Zhang, Xiao Zhou, Ziheng Zhao, Ya Zhang, Yanfeng Wang, and Weidi Xie. 2023. [Can gpt-4v\(ision\) serve medical applications? case studies on gpt-4v for multimodal medical diagnosis](#). *Preprint*, arXiv:2310.09909.
- Jinge Wu, Yunsoo Kim, and Honghan Wu. 2024. [Hallucination benchmark in medical visual question answering](#). *Preprint*, arXiv:2401.05827.

- Peng Xia, Kangyu Zhu, Haoran Li, Tianze Wang, Weijia Shi, Sheng Wang, Linjun Zhang, James Zou, and Huaxiu Yao. 2025. [Mmed-rag: Versatile multimodal rag system for medical vision language models](#). *Preprint*, arXiv:2410.13085.
- Justin Xu, Xi Zhang, Javid Abderezaei, Julie Bauml, Roger Boodoo, Fatemeh Haghighi, Ali Ganjizadeh, Eric Brattain, Dave Van Veen, Zaiqiao Meng, David W Eyre, and Jean-Benoit Delbrouck. 2025a. [RadEval: A framework for radiology text evaluation](#). In *Proceedings of the 2025 Conference on Empirical Methods in Natural Language Processing: System Demonstrations*, pages 546–557, Suzhou, China. Association for Computational Linguistics.
- Xinhao Xu, Hui Chen, Mengyao Lyu, Sicheng Zhao, Yizhe Xiong, Zijia Lin, Jungong Han, and Guiguang Ding. 2025b. [Mitigating hallucinations in multimodal large language models via image token attention-guided decoding](#). In *Proceedings of the 2025 Conference of the Nations of the Americas Chapter of the Association for Computational Linguistics: Human Language Technologies (Volume 1: Long Papers)*, pages 1571–1590, Albuquerque, New Mexico. Association for Computational Linguistics.
- Nur Yildirim, Hannah Richardson, Maria Teodora Wetscherek, Junaid Bajwa, Joseph Jacob, Mark Ames Pinnock, Stephen Harris, Daniel Coelho De Castro, Shruthi Bannur, Stephanie Hyland, Pratik Ghosh, Mercy Ranjit, Kenza Bouzid, Anton Schwaighofer, Fernando Pérez-García, Harshita Sharma, Ozan Oktay, Matthew Lungren, Javier Alvarez-Valle, and 2 others. 2024. [Multimodal healthcare ai: Identifying and designing clinically relevant vision-language applications for radiology](#). In *Proceedings of the CHI Conference on Human Factors in Computing Systems, CHI '24*, page 1–22. ACM.
- Shukang Yin, Chaoyou Fu, Sirui Zhao, Ke Li, Xing Sun, Tong Xu, and Enhong Chen. 2024. [A survey on multimodal large language models](#). *National Science Review*, 11(12):nwae403.
- Juan Manuel Zambrano Chaves, Shih-Cheng Huang, Yanbo Xu, Hanwen Xu, Naoto Usuyama, Sheng Zhang, Fei Wang, Yujia Xie, Mahmoud Khademi, Ziyi Yang, Hany Awadalla, Julia Gong, Houdong Hu, Jianwei Yang, Chunyuan Li, Jianfeng Gao, Yu Gu, Cliff Wong, Mu Wei, and 8 others. 2025. [A clinically accessible small multimodal radiology model and evaluation metric for chest x-ray findings](#). *Nature Communications*, 16(1).
- Xiaohua Zhai, Basil Mustafa, Alexander Kolesnikov, and Lucas Beyer. 2023. [Sigmoid loss for language image pre-training](#). *Preprint*, arXiv:2303.15343.
- Jiarui Zhang, Mahyar Khayatkhoei, Prateek Chhikara, and Filip Ilievski. 2025a. [Mllms know where to look: Training-free perception of small visual details with multimodal llms](#). *Preprint*, arXiv:2502.17422.
- Sheng Zhang, Yanbo Xu, Naoto Usuyama, Hanwen Xu, Jaspreet Bagga, Robert Tinn, Sam Preston, Rajesh Rao, Mu Wei, Naveen Valluri, Cliff Wong, Andrea Tupini, Yu Wang, Matt Mazzola, Swadheen Shukla, Lars Liden, Jianfeng Gao, Angela Crabtree, Brian Piening, and 5 others. 2025b. [Biomedclip: a multimodal biomedical foundation model pretrained from fifteen million scientific image-text pairs](#). *Preprint*, arXiv:2303.00915.
- Tianyi Zhang, Varsha Kishore, Felix Wu, Kilian Q. Weinberger, and Yoav Artzi. 2020. [Bertscore: Evaluating text generation with bert](#). *Preprint*, arXiv:1904.09675.
- Xi Zhang, Zaiqiao Meng, Jake Lever, and Edmond S. L. Ho. 2025c. [Libra: Leveraging temporal images for biomedical radiology analysis](#). In *Findings of the Association for Computational Linguistics: ACL 2025*, pages 17275–17303, Vienna, Austria. Association for Computational Linguistics.
- Xi Zhang, Zaiqiao Meng, Jake Lever, and Edmond SL Ho. 2024a. [Gla-ai4biomed at rrg24: Visual instruction-tuned adaptation for radiology report generation](#). In *Proceedings of the 23rd Workshop on Biomedical Natural Language Processing*, pages 624–634.
- Xiaoman Zhang, Julian Nicolas Acosta, Xiaoli Yang, Subathra Adithan, Luyang Luo, Hong-Yu Zhou, Joshua Miller, Ouwen Huang, Zongwei Zhou, Ibrahim Ethem Hamamci, Shruthi Bannur, Kenza Bouzid, Xi Zhang, Zaiqiao Meng, Aaron Nicolson, Bevan Koopman, Inhyeok Baek, Hanbin Ko, Mercy Prasanna Ranjit, and 3 others. 2025d. [Automated chest x-ray report generation remains unsolved](#). *Biocomputing 2026: Proceedings of the Pacific Symposium*, pages 236–250.
- Xiaoman Zhang, Hong-Yu Zhou, Xiaoli Yang, Oishi Banerjee, Julián N. Acosta, Josh Miller, Ouwen Huang, and Pranav Rajpurkar. 2024b. [Rexrank: A public leaderboard for ai-powered radiology report generation](#). *Preprint*, arXiv:2411.15122.
- Linxi Zhao, Yihe Deng, Weitong Zhang, and Quanquan Gu. 2025. [Mitigating object hallucination in large vision-language models via image-grounded guidance](#). *Preprint*, arXiv:2402.08680.
- Weike Zhao, Chaoyi Wu, Xiaoman Zhang, Ya Zhang, Yanfeng Wang, and Weidi Xie. 2024. [RaTEScore: A metric for radiology report generation](#). In *Proceedings of the 2024 Conference on Empirical Methods in Natural Language Processing*, pages 15004–15019, Miami, Florida, USA. Association for Computational Linguistics.
- Zhihong Zhu, Yunyan Zhang, Xianwei Zhuang, Fan Zhang, Zhongwei Wan, Yuyan Chen, QingqingLong QingqingLong, Yefeng Zheng, and Xian Wu. 2025. [Can we trust AI doctors? a survey of medical hallucination in large language and large vision-language models](#). In *Findings of the Association for Computational Linguistics: ACL 2025*, pages 6748–6769, Vienna, Austria. Association for Computational Linguistics.

Appendix Contents

A Related Work	15
A.1 Radiology Multimodal Large Language Models	15
A.2 Medical Hallucination in Multimodal Large Language Models . .	15
A.3 Radiology Report Generation	16
A.4 Contrastive Decoding Strategies	16
B Research Objectives	16
B.1 Research Aims	16
B.2 Research Scope	16
C Datasets and Metrics	17
C.1 Datasets Description	17
C.2 Evaluation Metrics	17
D Experimental Details	18
D.1 Backbone Models	18
D.2 Method Configuration	19
D.3 Expert Model Setting	19
E Additional Experimental Results	19
E.1 Comparison of Decoding Strategies on Radiology Report Generation	19
E.2 Comparison of Backbone MLLMs for Radiology Report Generation .	21
E.3 Alternative Backbone MLLMs for Visual Question Answering	22
F Additional Ablation Studies	23
F.1 Ablation of Guidance Strength in Clinical Contrastive Decoding . .	23
F.2 Robustness Test of Clinical Contrastive Decoding with Random Prior	24
F.3 Evaluation of Clinical Contrastive Decoding on Additional Label Types	25
G Balancing Accuracy and Ambiguity	25
H Extended Discussion on Limitations	26
I Additional Statement	27

A Related Work

A.1 Radiology Multimodal Large Language Models

Substantial advancements have been made in applying MLLMs to radiology, particularly for generating narrative-style reports directly from medical images (Sharma et al., 2025b; Zhang et al., 2025c). This trend highlights the need for domain-specific MLLMs that can support clinical workflows, reduce the workload of radiologists, and improve patient care (Huang et al., 2023; Wu et al., 2023). Recent models such as Med-PaLM M (Tu et al., 2023), MAIRA-1 (Hyland et al., 2024), Lingshu (Team et al., 2025), and Med-Gemma (Sellergren et al., 2025) have made encouraging progress. However, medical hallucination remains a key limitation, compromising the clinical reliability of MLLMs (Kim et al., 2025).

A.2 Medical Hallucination in Multimodal Large Language Models

Hallucination in LLMs is commonly defined as generating content that is irrelevant or unfaithful to the input (Tonmoy et al., 2024). In MLLMs, this often manifests as object hallucination, where generated outputs contradict the visual or factual evidence (Sahoo et al., 2024). Unlike general-domain applications, the medical domain presents unique triggers for hallucinations, such as clinically implausible prompts or subtle finding cues, and exhibits a markedly lower tolerance for errors (Wang et al., 2025b). The recent survey by Zhu et al. (2025) examines the causes of medical hallucinations and reviews current mitigation strategies. Among various contributing factors, strict privacy regulations exacerbate the scarcity and imbalance of clinical training data (Jiang et al., 2025a), which is a key cause of medical hallucinations and often more critical than factors introduced during training or inference (Hager et al., 2024). Corresponding mitigation strategies primarily focus on training-time interventions, such as constructing datasets that reflect a coherent chain of diagnostic reasoning (Lai et al., 2025), followed by post-training (Banerjee et al., 2024) or deployment with retrieval-augmented generation (RAG) (Sun et al., 2025). At inference time, voting-based mechanisms have been adopted to improve accuracy in VQA (Liu et al., 2024c), but these approaches do not generalise well to the more complex radiology report generation (RRG) task.

A.3 Radiology Report Generation

RRG aims to generate free-text descriptions of clinical findings, establishing it as a central objective in automated medical imaging analysis (Wang et al., 2018; Zhang et al., 2024a). Recent efforts in RRG have primarily focused on improving the quantity and quality of training data to reduce medical hallucinations (Zhang et al., 2025d). LLaVA-Rad (Zambrano Chaves et al., 2025) uses an API-based model to sanitise noisy clinical sections, while retrieval-augmented generation has been explored to improve factual grounding (Li et al., 2024; Hou et al., 2025). Advanced models, MAIRA-2 (Bannur et al., 2024) integrates structured clinical sections and prior reports to improve diagnostic grounding, while Libra (Zhang et al., 2025c) mitigates temporal hallucinations by explicitly modelling historical image information. However, these approaches often require costly retraining, extensive dataset curation, and may raise privacy or security concerns. They also rely on retrieval infrastructure, which limits their practicality in out-of-distribution settings or when adapting to new benchmarks.

A.4 Contrastive Decoding Strategies

Contrastive decoding has emerged as an effective inference-time approach to mitigate hallucinations in generative models (Leng et al., 2023; Favero et al., 2024), offering a lightweight alternative to costly training-time interventions. Visual Contrastive Decoding (VCD) (Leng et al., 2023) addresses object hallucinations by comparing output distributions between original and distorted visual inputs. Similarly, Instruction Contrastive Decoding (ICD) (Wang et al., 2024b) explores hallucination amplification under perturbed textual instructions. Alternative inference-time methods, such as VTI (Liu et al., 2024d), OPERA (Huang et al., 2024), M3ID (Favero et al., 2024), and DeCo (Wang et al., 2025a), guide generation using shallow visual cues, fixed transformer layers, or token-level confidence scores. Recent work, such as Attn-Lens (Jiang et al., 2025b), achieves state-of-the-art performance in general-domain settings by integrating information across multiple attention heads. While effective in such domains, these methods struggle to mitigate medical hallucinations in radiology, partly due to the grayscale nature of imaging data and the scarcity of diverse, domain-specific datasets (Singhal et al., 2023). Moreover, radiology MLLMs are often trained for single tasks

(RRG or VQA), which limits the generalisability of training-free strategies in clinical applications.

B Research Objectives

B.1 Research Aims

This work introduces Clinical Contrastive Decoding (**CCD**), a plug-and-play, inference-time framework designed to mitigate medical hallucinations in radiology multimodal large language models (MLLMs). The primary objective is to reduce clinically harmful errors, particularly prompt-induced hallucinations (Chen et al., 2024b), without modifying model parameters or requiring additional training. **CCD** enhances output reliability by integrating expert signals, such as predictions from pretrained pathology classifiers, during the decoding process. Designed to be model-agnostic, it applies broadly across MLLM architectures and tasks, including RRG and VQA.

To facilitate a fair comparison, it is also important to clarify what this work does not aim to address. We do not propose new model architectures or novel training methodologies. Our focus is on test-time decoding. Therefore, we do not compare with approaches that involve architectural modifications, additional training, or retrieval-based augmentation requiring external corpora. Nor do we attempt to eliminate all forms of medical hallucination. Instead, our focus is on reducing prompt-induced hallucinations that carry clinical importance or potential risk. Even the mitigation of a subset of hallucinations can lead to meaningful gains in overall task performance. For instance, in the case of view-type VQA tasks, symptom-guided decoding enables models to answer more accurately. This is because most findings are concentrated in frontal chest X-rays, while lateral views provide less diagnostic signal for common conditions (Bannur et al., 2024). As a result, expert-derived symptom likelihoods help the model infer appropriate view type even when it is not explicitly stated in the question.

B.2 Research Scope

This study is restricted to the use of pretrained radiology-focused MLLMs for medical imaging tasks involving chest X-rays, which represent the most commonly used imaging modality in clinical practice. All experiments are conducted using only frontal-view chest radiographs, specifically

anterior-posterior (AP) and posterior-anterior (PA) projections. We focus on two downstream tasks: radiology report generation (RRG) and visual question answering (VQA). The backbone models evaluated in this work include MAIRA-2 (Bannur et al., 2024), Libra (Zhang et al., 2025c), LLaVA-Rad (Zambrano Chaves et al., 2025), and LLaVA-Med (Li et al., 2023a). These models are used without any additional finetuning. For external guidance, we incorporate predictions from pretrained image-level expert models, either supervised classifiers (e.g., DenseNet from TorchXRyVision (Cohen et al., 2021)) or zero-shot vision-language models (e.g., MedSigLIP (Selligren et al., 2025)), that estimate the presence of clinical findings.

Several important areas are intentionally excluded from the scope of this work. We do not address other medical imaging modalities such as computed tomography (CT), magnetic resonance imaging (MRI), or ultrasound. Our framework does not incorporate multi-modality signals derived from clinical notes, laboratory values, or electronic health records (EHRs). Our scope is restricted to hallucinations arising in radiology-specific MLLMs, and does not extend to general-domain MLLMs. In particular, we focus on prompt-induced hallucinations, a critical and under-addressed subset of medical hallucinations. Furthermore, post-processing techniques such as output filtering, retrieval augmentation, or report rewriting are outside the focus of this study. The proposed CCD method operates entirely at inference time and does not require model retraining, which ensures compatibility with a wide range of pretrained models while maintaining low deployment overhead.

C Datasets and Metrics

C.1 Datasets Description

MIMIC-CXR (Johnson et al., 2019b) A large-scale, publicly available dataset comprising 377,110 chest radiographs from 227,835 imaging studies, each paired with a free-text radiology report. We make use of the JPEG images from the MIMIC-CXR-JPG release (Johnson et al., 2019a), which are derived from the original DICOM files. To ensure consistency, only anterior-posterior (AP) or posterior-anterior (PA) frontal views are retained.

Each report is preprocessed to extract five clinically relevant sections: *Findings*, *Indication*, *Tech-*

nique, *Comparison*, and *History*. This is done using pattern-matching heuristics based on the official preprocessing scripts (Johnson et al., 2018). We evaluate on the official test split, which consists of 2,461 studies that contain frontal-view images and non-empty “Findings” sections.

IU-Xray (Demner-Fushman et al., 2015) A publicly available dataset for medical image analysis, consisting of 7,470 chest X-ray images and 3,955 corresponding diagnostic reports. To ensure compatibility with both MLLMs and expert models, all images are converted to PNG format. For evaluation, we select 3,307 frontal-view cases that include non-empty “Findings” sections.

CheXpert Plus (Chambon et al., 2024) A large-scale dataset comprising 223,462 image-report pairs from 187,711 studies across 64,725 patients. Since the official test split is not publicly available, we use the validation set, which includes 72 frontal-view samples with non-empty “Findings” sections for evaluation on the report generation task.

Medical-CXR-VQA (Hu et al., 2024) A large-scale visual question answering dataset derived from MIMIC-CXR, focusing exclusively on antero-posterior (AP) and postero-anterior (PA) chest X-ray views. It includes six predefined question types: *abnormality*, *location*, *type*, *level*, *view*, and *presence*. We use only the official test split, which contains 78,124 image-question pairs.

C.2 Evaluation Metrics

Lexical Metrics We employ commonly used natural language metrics to assess the textual overlap between generated and reference reports. Specifically, ROUGE-L (Lin, 2004) measures the length of the longest common subsequence, BLEU (Papineni et al., 2002) computes n-gram precision with a brevity penalty, and BERTScore (Zhang et al., 2020) leverages contextual embeddings from BERT (Devlin et al., 2019) to assess semantic similarity. All metrics are computed with their default configurations. For BLEU, we report results using BLEU-4 (i.e., n=4), following prior work.

Clinical Metrics We adopt several radiology-specific metrics to evaluate the clinical relevance and accuracy of generated reports. RadGraph-F1 (Delbrouck et al., 2022) parses reports into structured graphs composed of clinical entities (e.g.,

anatomical sites and observations) and their relations. Temporal-F1 (Zhang et al., 2025c) extends this by assessing the correctness of temporal descriptors such as “worsened,” “improved,” or “stable.” RaTeScore (Zambrano Chaves et al., 2025) focuses on critical diagnostic concepts and anatomical details, offering robustness to medical synonyms and sensitivity to negation cues. RadEval-BERT (Xu et al., 2025a) leverages a radiology-adapted ModernBERT model (Warner et al., 2024) to assess semantic similarity between generated and reference reports. CheXbert-F1 (Smit et al., 2020) applies an automatic labeler to extract “present,” “absent,” or “uncertain” labels for 14 clinical conditions (Irvin et al., 2019); we report both the full 14-class F1 score and a 5-class variant focusing on common pathologies (*Atelectasis*, *Cardiomegaly*, *Consolidation*, *Edema*, and *Pleural Effusion*).

To ensure fairness, reproducibility, and consistency with prior work, all lexical and clinical evaluation metrics are computed using the RadEval (Xu et al., 2025a) toolkit, with each metric applied using its default configuration.

VQA Evaluation For the visual question answering (VQA) task, we report micro-averaged Recall and F1 scores, computed based on whether ground-truth labels are present in the generated responses. Since the model outputs are in free-form natural language (e.g., “There is evidence of opacity in the left lung.”), and the ground truth is a structured label list (e.g., “atelectasis, opacity”), we only assess whether each reference label is mentioned in the generated text.

Specifically, true positives are counted as ground-truth labels that appear in the output, and false negatives are those that are missing. False positives are not penalised, as it is inherently difficult to determine which additional labels in a free-text sentence constitute hallucinations. This formulation aligns well with the clinical objective of ensuring that critical findings are not missed.

We adopt micro-averaging across all samples to reflect the overall coverage and correctness of label inclusion. Compared to macro-averaging, micro-averaging gives appropriate weight to frequent conditions and avoids over-penalising rare labels in sparse multi-label settings. This makes micro Recall and F1 the most suitable metrics for evaluating free-text VQA responses in radiology.

D Experimental Details

In this section, we provide additional details about the four backbone MLLMs used in our experiments, along with the decoding strategies and expert model configurations. All experiments are conducted on two NVIDIA RTX 3090 GPUs (24GB memory each) with BF16 precision enabled. Since CCD is a fully test-time decoding strategy, it requires no additional training and can be applied directly to any pretrained MLLM. Despite incorporating an expert model and a two-stage decoding process, it maintains a lightweight deployment cost. On average, CCD incurs an inference-time overhead of approximately $1.45\times$ relative to standard greedy decoding. The actual runtime may vary depending on hardware configurations, particularly the floating-point operations per second (FLOPS) supported by the GPU.

D.1 Backbone Models

MAIRA-2 (Bannur et al., 2024) A model developed specifically for grounded radiology report generation, where the goal is not only to produce clinically accurate reports but also to localise findings within the image. The model is built upon the LLaVA framework (Liu et al., 2023), and incorporates a frozen Rad-DINO-MAIRA-2 vision encoder (Pérez-García et al., 2024), a Vicuna-7B (Chiang et al., 2023) language backbone, and a 4-layer MLP that facilitates cross-modal alignment between image features and language representations.

To ensure fair and consistent evaluation, the chat templates and system prompts provided in the HuggingFace ⁶ implementation of MAIRA-2 are disabled, as they include engineering optimisations not described in the original paper. Instead, unified default instructions are applied to all models.

Libra (Zhang et al., 2025c) A temporally-informed multimodal model designed for generating the *Findings* section in chest X-ray reports. Distinct from traditional single-image approaches, Libra processes longitudinal image pairs to capture disease evolution. It integrates a frozen Rad-DINO (Pérez-García et al., 2025) encoder with Meditron-7B (Chen et al., 2023), linked through a Temporal Alignment Connector. This connector incorporates a Layerwise Feature Extractor and a Temporal Fusion Module to encode multi-scale visual changes into a unified representation.

⁶<https://huggingface.co/microsoft/maira-2>

LLaVA-Rad (Zambrano Chaves et al., 2025)

An instruction-tuned multimodal model designed for radiology report generation. It builds upon the LLaVA (Liu et al., 2023) architecture and employs LoRA (Hu et al., 2021) for parameter-efficient fine-tuning. To reduce training cost, the model is trained exclusively on MIMIC-CXR data, which offers high-quality radiology reports. These reports are further refined using GPT-4 (OpenAI et al., 2024) structuring to enhance label clarity and consistency. For visual encoding, LLaVA-Rad adopts a Biomed-CLIP (Zhang et al., 2025b) model pretrained on biomedical image-text pairs, improving domain alignment with radiological content.

LLaVA-Med (Li et al., 2023a) A biomedical adaptation of the LLaVA (Liu et al., 2023) model, trained on a large-scale synthetic instruction-following dataset generated from PMC-15M (Zhang et al., 2025b) image-text pairs. Instructions are automatically generated using GPT-4 (OpenAI et al., 2024) without manual annotation. The model is finetuned in two stages: first aligning on biomedical image-text data, then learning open-ended instruction following. We use version 1.5 of LLaVA-Med, which adopts Mistral-7B (Jiang et al., 2023) as the language model and includes a jointly trained CLIP image encoder (Radford et al., 2021). This version is well-suited for biomedical VQA tasks, effectively handling clinical questions and extracting relevant findings from chest X-rays.

CheXagent (Chen et al., 2024c) An instruction-tuned foundation model designed specifically for chest X-ray understanding. The model combines a dedicated vision backbone with a cross-modal alignment module to effectively integrate visual features and textual instructions. It is trained on CheXinstruct (Chen et al., 2024c), a comprehensive instruction corpus constructed by unifying data from 28 publicly available medical datasets, covering a wide range of radiological reasoning tasks.

In this work, we adopt the 8B variant of CheXagent as a strong baseline for visual question answering. According to the original report, this model demonstrates stronger baseline performance than LLaVA-Med on multiple chest X-ray VQA benchmarks, making it a suitable candidate for evaluating the robustness and generality of our method under a stronger backbone.

D.2 Method Configuration

Since the MAIRA-2 (Bannur et al., 2024) model largely follows the LLaVA architecture (Liu et al., 2023), with the main differences being the use of a specialised image encoder and a four-layer fully connected multi-layer perceptron for vision-language alignment, we apply each training-free decoding method using the default LLaVA-type settings specified in its original publication. All comparison methods are implemented according to their published hyperparameter recommendations to enable fair and consistent evaluation. We do not perform any additional tuning of these hyperparameters beyond what is reported in the respective works. A summary of these decoding methods is provided in Appx. E.1.

D.3 Expert Model Setting

For the DenseNet model provided by TorchXRyVision (Cohen et al., 2021), we adopt the CheXpert Pathology Classifier, which is pretrained on the CheXpert dataset (Irvin et al., 2019). This model outputs probability scores for each of the 14 predefined pathologies, with label smoothing applied around the 0.5 threshold to enhance prediction stability. These confidence scores are directly used as expert guidance signals within our CCD framework.

For MedSigLIP (Sellergren et al., 2025), a concurrent and publicly released variant of SigLIP (Zhai et al., 2023) tailored to encode medical images and text into a shared embedding space, we perform zero-shot classification over a predefined list of symptom labels following the official instruction format. Each prediction is based on a pair of textual prompts, such as “a chest X-ray with Atelectasis” and “a chest X-ray with no Atelectasis.” By comparing the model’s confidence scores for these alternatives, we obtain the probability associated with the positive prompt, which indicates the likelihood of the symptom being present in the image. These probabilities are then used as expert-derived guidance signals in the CCD module.

E Additional Experimental Results

E.1 Comparison of Decoding Strategies on Radiology Report Generation

To provide a more comprehensive evaluation of CCD in comparison with other training-free hallucination mitigation methods, we expand upon the analysis in Sec. 4.2 by including an additional set

of recent approaches. In total, we evaluate against eleven training-free methods under the same experimental settings. **The following is a brief overview of these methods.**

VCD (Leng et al., 2023) introduces contrastive decoding by comparing the output distributions from original and perturbed images. This approach reduces over-reliance on dataset priors and unimodal statistical biases. M3ID (Favero et al., 2024) amplifies the influence of visual inputs during decoding, encouraging the model to generate tokens with higher visual-text mutual information. AVISC (Woo et al., 2025) detects visually misaligned tokens by examining attention patterns and dynamically refines the next-token prediction by contrasting logits from original versus visually-blinded inputs. OPERA (Huang et al., 2024) introduces a decoding-time penalty on logits to curb overconfidence, combined with a rollback mechanism that reviews earlier summary tokens and reallocates selections when needed. ICD (Wang et al., 2024b) contrasts the distributions from standard and instruction-perturbed inputs to amplify alignment uncertainty and effectively suppress hallucinated concepts embedded in the original distribution. PAI (Liu et al., 2024e) intervenes in the inference stage to steer the decoding process toward the original image perception direction, primarily by adjusting the self-attention heads in the decoder layers of MLLMs. VTI (Liu et al., 2024d) steers the latent space representations during inference to stabilise vision features, thereby reducing hallucinations. DeCo (Wang et al., 2025a) adaptively selects preceding layers and proportionally fuses their information into the final layer to dynamically adjust output logits. VISTA (Li et al., 2025b) mitigates hallucinations by combining two strategies: strengthening visual information in the activation space and utilising early-layer activations to guide more semantically coherent decoding. AttnLens (Jiang et al., 2025b) mitigates hallucinations by refining visual attention through the aggregation of signals from multiple attention heads. MARINE (Zhao et al., 2025) addresses object hallucinations by incorporating image-grounded guidance only at the prompt level into the decoding process. In our evaluation, we adopt the *MARINE-Truth* setting, using ground-truth labels of thoracic structures such as the lungs, heart, and pleural cavity as grounded references.

Additionally, in the general domain, numerous recent **training-free** methods have been proposed

to mitigate hallucinations in MLLMs. These methods are publicly available and widely used within the research community. However, their underlying task assumptions are often incompatible with radiology-specific generation settings. For example, methods such as VDGD (Ghosh et al., 2025) first prompt an MLLM to generate a textual description of the image, which is then concatenated as a prefix to the original prompt. Similarly, SumGD (Min et al., 2025) constructs summarised instructions to guide the model prior to decoding. These types of strategies are not applicable to radiology models, which are often instruction-tuned for tasks such as radiology report generation. Since the report itself serves as a detailed image description, adding a separate generated caption will introduce redundancy or interfere with the model’s instruction-following behaviour.

While some methods, such as FarSight (Tang et al., 2025) and iTaD (Xu et al., 2025b), focus heavily on improving caption generation, their design motivations are largely driven by issues such as attention collapse, positional information decay, and the progressive reduction of attention weights to image tokens as model depth increases. However, these issues are less relevant for tasks such as visual question answering (VQA), which typically require only short, discrete responses. Consequently, such methods are not directly applicable to VQA settings.

Furthermore, some methods attempt to mitigate hallucinations by refining the visual input. For instance, ViCrop (Zhang et al., 2025a) performs automatic visual cropping to select important patch tokens, which are then re-concatenated with the original image tokens for generation. DyFo (Li et al., 2025a) leverages grounding-based visual expert models, such as Grounding DINO, to conduct visual search and eliminate object-level hallucinations. AGLA (An et al., 2025) uses adaptive masks to select relevant image patches as visual prompts, while masking out irrelevant regions. While these approaches have shown promising results in the general domain, their applicability to radiology is also limited. This is primarily due to the lack of strong pretrained grounding models in the medical domain, as well as the use of single-channel grayscale chest X-rays instead of three-channel natural images, which constrains the applicability of visual prompt strategies in this setting.

In contrast to the methods discussed above, our proposed approach is more suitable for radiology

Method	Lexical Metric			Clinical Metric					
	ROUGE-L	BLEU	BERTScore	RadGraph-F1	Temporal-F1	RaTEScore	RadEval-BERT	CheXbert ⁵ _{F1}	CheXbert ¹⁴ _{F1}
MIMIC-CXR									
Baseline	19.57	1.61	49.56	16.23	12.11	50.82	16.96	16.14	10.57
+ VCD	19.47	<u>2.02</u>	48.99	15.90	12.57	49.85	<u>17.49</u>	19.17	15.47
+ M3ID	14.45	1.50	41.11	11.85	13.35	43.77	15.87	22.34	10.16
+ AVISC	<u>19.68</u>	1.94	49.28	15.80	12.49	50.04	17.39	16.17	12.84
+ OPERA	19.18	1.77	49.31	16.06	13.26	50.59	17.09	16.25	11.82
+ ICD	17.43	<u>2.02</u>	46.58	13.65	13.98	47.01	17.13	17.25	12.26
+ PAI	18.46	1.68	49.13	16.24	<u>13.99</u>	50.51	16.93	17.59	12.69
+ VTI	19.21	1.68	49.77	<u>16.42</u>	13.48	<u>51.20</u>	16.87	12.13	8.75
+ DeCO	19.40	1.65	49.33	15.93	12.95	50.65	17.27	16.60	11.57
+ VISTA	10.98	0.80	36.59	6.43	13.61	38.94	16.84	<u>26.28</u>	<u>15.82</u>
+ Attn-Lens	19.51	1.68	<u>49.67</u>	16.37	13.45	50.86	17.15	16.74	10.98
+ MARINE	18.88	1.62	48.92	14.59	8.97	50.43	17.09	8.37	5.91
+ CCD	20.70	2.10	51.62	19.01	17.58	53.32	17.50	27.05	16.02
IU-Xray									
Baseline	18.50	2.67	42.19	16.52	66.06	46.86	20.15	4.02	24.14
+ CCD	20.77	3.31	46.25	21.12	67.16	50.47	22.14	19.96	28.23
CheXpert Plus									
Baseline	18.07	1.83	45.91	14.27	22.78	47.47	1.99	13.54	8.39
+ CCD	18.59	1.84	46.64	14.89	32.04	47.55	2.91	14.76	9.75

Table 5: **Comparison of report generation performance across decoding methods.** MAIRA-2 (Bannur et al., 2024), the top open-source model on the ReXrank (Zhang et al., 2024b) leaderboard, is used as the baseline. Results on IU-Xray and CheXpert Plus are reported only for our method. **Best** and second-best results are bolded and underlined, respectively.

MLLMs and the tasks defined within this setting. As shown in Table 5, the results reaffirm our earlier findings that CCD consistently improves the performance of backbone models across both lexical and clinical evaluation metrics. To further evaluate the clinical effectiveness of CCD, we additionally adopt the GREEN framework (Ostmeier et al., 2024) for both quantitative and qualitative assessment. GREEN leverages the natural language understanding capabilities of language models to identify and explain clinically significant errors in radiology reports. On MIMIC-CXR with the RRG task, the MAIRA-2 baseline achieves a GREEN score of 18.03. After applying CCD, the score increases to 19.14 ($\uparrow 1.11$, $\approx 6\%$, indicating better clinical alignment in the generated reports).

In summary, these results show that CCD is more effective for radiology-specific generation tasks than general-domain strategies, particularly for chest X-ray interpretation. This highlights its advantages in incorporating domain-specific knowledge into the decoding process.

E.2 Comparison of Backbone MLLMs for Radiology Report Generation

In addition to MAIRA-2 (Bannur et al., 2024), we evaluate CCD on several other MLLMs to assess its generalisability in the radiology report generation task. These include Libra (Zhang et al., 2025c) and LLaVA-Rad (Zambrano Chaves et al., 2025), which are specifically tailored for the RRG task, as well as LLaVA-Med (Li et al., 2023a), a domain-specific foundation MLLM. We evaluate these models on three datasets: MIMIC-CXR (Johnson et al., 2019b), IU-Xray (Demner-Fushman et al., 2015), and CheXpert Plus (Chambon et al., 2024). Importantly, we do not tune the control strength hyperparameters of CCD. All models are evaluated using the default CCD settings, which may under-optimize performance for certain backbones.

As shown in Table 6, applying CCD consistently improves overall performance across all backbones, particularly in terms of clinical metrics. Interestingly, we observe that improvements in clinical consistency may occasionally come at the cost of lexical quality. For instance, LLaVA-Med exhibits a $1.64\times$ gain in the CheXbert⁵_{F1}, but also shows slight decreases in lexical metrics. This suggests

Method	Lexical Metric			Clinical Metric					
	ROUGE-L	BLEU	BERTScore	RadGraph-F1	Temporal-F1	RaTEScore	RadEval-BERT	CheXbert ⁵ _{F1}	CheXbert ¹⁴ _{F1}
MIMIC-CXR									
LLaVA-Med	15.60	0.95	38.19	7.59	13.65	43.91	17.53	25.78	21.89
+ CCD	15.00 ↓	0.65 ↓	35.00 ↓	8.07 ↑	13.87 ↑	46.05 ↑	17.57 ↑	42.30 ↑	33.14 ↑
LLaVA-Rad	25.03	8.06	53.32	22.35	22.11	53.97	28.37	58.21	54.48
+ CCD	25.32 ↑	7.43 ↓	54.24 ↑	23.52 ↑	22.59 ↑	55.70 ↑	28.30 ↓	58.22 ↑	54.63 ↑
Libra	21.50	4.74	50.52	20.46	19.59	53.13	24.99	59.46	51.76
+ CCD	24.18 ↑	6.26 ↑	53.06 ↑	22.65 ↑	19.88 ↑	55.30 ↑	25.82 ↑	60.02 ↑	52.78 ↑
IU-Xray									
LLaVA-Med	11.94	0.39	34.58	7.14	60.23	43.02	20.12	7.71	5.44
+ CCD	11.52 ↓	0.29 ↓	31.85 ↓	7.35 ↑	49.00 ↓	43.05 ↑	19.55 ↓	18.75 ↑	8.13 ↑
LLaVA-Rad	21.07	4.18	48.37	22.42	32.99	56.66	21.07	42.11	47.50
+ CCD	25.36 ↑	5.62 ↑	56.38 ↑	31.73 ↑	36.80 ↑	64.94 ↑	23.24 ↑	42.48 ↑	47.56 ↑
Libra	24.31	2.99	51.59	26.38	59.06	56.22	23.63	43.86	45.46
+ CCD	24.27 ↓	4.44 ↑	50.92 ↓	26.47 ↑	62.07 ↑	58.67 ↑	24.74 ↑	44.05 ↑	45.53 ↑
CheXpert Plus									
LLaVA-Med	14.40	0.72	32.59	4.63	25.00	42.16	4.63	25.84	25.00
+ CCD	14.45 ↑	0.84 ↑	33.78 ↑	8.49 ↑	28.09 ↑	44.58 ↑	2.71 ↓	29.84 ↑	26.40 ↑
LLaVA-Rad	18.94	2.67	43.31	17.13	14.36	47.14	6.67	51.96	50.93
+ CCD	19.43 ↑	2.66 ↓	47.16 ↑	17.81 ↑	23.89 ↑	50.31 ↑	6.73 ↑	51.99 ↑	51.37 ↑
Libra	18.87	2.14	47.04	19.20	27.18	49.33	7.58	45.68	50.08
+ CCD	19.87 ↑	3.23 ↑	48.03 ↑	20.15 ↑	30.91 ↑	49.38 ↑	7.85 ↑	46.75 ↑	50.21 ↑

Table 6: **Overall performance on the radiology report generation task.** Our method is compared with baselines that use greedy decoding without any clinical section input. “↑” indicates improvement, “↓” denotes degradation relative to the baseline.

Model	Question Classification												Overall	
	Abnormality		Presence		View		Location		Level		Type			
	F1	Recall	F1	Recall	F1	Recall	F1	Recall	F1	Recall	F1	Recall	F1	Recall
CheXagent-8B	61.75	45.74	68.18	59.40	38.28	23.97	7.67	3.99	27.24	15.77	8.54	4.46	47.67	33.12
+ CCD	62.28 ↑	45.22 ↓	68.83 ↑	52.47 ↓	39.89 ↑	24.91 ↑	9.93 ↑	5.23 ↑	42.50 ↑	26.99 ↑	8.77 ↑	4.59 ↑	51.15 ↑	34.36 ↑

Table 7: **Performance of CCD on the Medical Visual Question Answering with CheXagent-8B** “↑” indicates improvement, “↓” denotes degradation relative to the baseline.

that choosing appropriate hyperparameters for each model is critical to achieving a balanced trade-off between lexical and clinical performance. Overall, these results support the general applicability of CCD in enhancing radiology MLLMs across different architectures and evaluation settings, consistent with the conclusions drawn in Sec. 4.2.

E.3 Alternative Backbone MLLMs for Visual Question Answering

In this section, we further analyse the VQA performance of models with different backbone capacities. Following the same experimental settings as in Sec. 4.3 and Table 3, we further evaluate the generalisability of CCD using an alternative model,

CheXagent-8B (Chen et al., 2024c). This model is an instruction-tuned foundation model for chest X-ray interpretation and integrates a vision encoder with a cross-modal adapter to align visual and textual representations.

As shown in Table 7, CCD improves F1 scores across all evaluated categories and achieves better overall performance compared to the baseline. For specific categories such as *abnormality* and *presence*, we observe a moderate decrease in recall accompanied by a notable increase in precision, resulting in an overall gain in F1 score. This suggests that the model becomes more cautious in its predictions, producing fewer false positives while preserving overall reliability.

α	Lexical Metric			Clinical Metric					
	ROUGE-L	BLEU	BERTScore	RadGraph-F1	Temporal-F1	RaTEScore	RadEval-BERT	CheXbert _{F1} ⁵	CheXbert _{F1} ¹⁴
0.00	18.22	1.26	49.40	16.71	13.81	51.59	16.65	19.02	12.06
0.25	19.71	1.49	50.73	17.56	15.49	52.68	16.95	16.89	10.52
0.50	20.70	2.10	51.62	19.01	17.58	53.32	17.50	27.05	16.02
0.75	<u>20.89</u>	<u>2.59</u>	<u>51.80</u>	18.36	<u>17.53</u>	<u>53.03</u>	18.36	<u>33.00</u>	21.36
1.00	20.95	2.94	51.69	<u>18.45</u>	17.12	52.82	<u>18.25</u>	33.54	<u>17.73</u>

Table 8: **Ablation study of the α hyperparameter.** $\beta = 0.5$ and $\gamma = 10$ are used as default values. **Best** and **second-best** results are bolded and underlined, respectively. $\alpha \in [0, 1]$.

β	Lexical Metric			Clinical Metric					
	ROUGE-L	BLEU	BERTScore	RadGraph-F1	Temporal-F1	RaTEScore	RadEval-BERT	CheXbert _{F1} ⁵	CheXbert _{F1} ¹⁴
0.00	20.73	1.96	51.72	18.78	17.40	53.21	17.71	21.02	11.47
0.25	<u>20.72</u>	2.02	<u>51.65</u>	18.83	<u>17.54</u>	<u>53.30</u>	<u>17.54</u>	22.68	12.69
0.50	20.70	2.10	51.62	19.01	17.58	53.32	17.50	27.05	16.02
0.75	20.51	2.05	51.43	<u>18.97</u>	17.18	53.23	17.53	28.42	<u>17.95</u>
1.00	19.85	<u>2.07</u>	50.83	18.64	16.37	53.03	17.47	<u>28.15</u>	19.65

Table 9: **Ablation study of the β hyperparameter.** $\alpha = 0.5$ and $\gamma = 10$ are used as default values. **Best** and **second-best** results are bolded and underlined, respectively. $\beta \in [0, 1]$.

Moreover, employing a stronger backbone such as CheXagent-8B helps mitigate the modest declines observed in the *Location* and *Type* categories (see Appx. G), suggesting that improved base model capacity can complement CCD’s effectiveness across question types. This is particularly beneficial in cases where expert models offer limited coverage of fine-grained radiological signals, such as lesion morphology or spatial localisation, which may otherwise bias the guidance process.

F Additional Ablation Studies

F.1 Ablation of Guidance Strength in Clinical Contrastive Decoding

To understand the impact of guidance strength in CCD, we perform ablation studies by varying its three control hyperparameters (α , β , and γ). In each experiment, we vary one hyperparameter while keeping the other two fixed, allowing us to isolate its effect on generation performance. These hyperparameters regulate the balance between the original MLLM output and the guidance from the clinical expert, determining how much influence each component has on the final generation. All experiments are conducted using MAIRA-2 (Bannur et al., 2024) as the backbone model, evaluated on the MIMIC-CXR (Johnson et al., 2019b) dataset for the radiology report generation task.

Effect of α on Guidance Strength As shown in Table 8, we investigate the effect of varying

α , which controls the overall guidance strength in the first stage of Symptom-grounded Contrastive Decoding. Increasing α strengthens the model’s reliance on labels provided by the expert model to suppress false negatives. We observe that as α increases from 0 to 1, both lexical metrics and CheXbert-based scores consistently improve. However, other metrics such as RadGraph-F1 and RaTeScore begin to degrade once α exceeds 0.5.

This suggests that while stronger anchor label guidance can enhance entity coverage and clinical consistency, it may also result in overly verbose generations. Specifically, setting $\alpha = 1$ causes the model to fully rely on the initial expert-provided anchor, producing detailed descriptions that include more symptom labels and semantic content than necessary. To balance lexical fluency and clinical accuracy, we adopt $\alpha = 0.5$ as the default setting.

Effect of β on Guidance Strength As shown in Table 9, we investigate the effect of varying β , which controls the overall guidance strength in the second stage of Expert-informed Contrastive Decoding. Increasing β corresponds to stronger reliance on the expert model’s confidence scores, aiming to reduce false positives. We observe that as β increases, clinical metrics, especially the CheXbert-based scores, consistently improve. However, lexical scores follow the opposite trend and gradually decrease. In addition, RadGraph-F1, Temporal-F1, and RaTeScore decline when β exceeds 0.5.

γ	Lexical Metric			Clinical Metric					
	ROUGE-L	BLEU	BERTScore	RadGraph-F1	Temporal-F1	RaTEScore	RadEval-BERT	CheXbert _{F1} ⁵	CheXbert _{F1} ¹⁴
2	<u>20.70</u>	1.98	<u>51.65</u>	18.85	17.52	<u>53.32</u>	<u>17.56</u>	22.20	12.45
5	20.71	2.05	51.67	<u>18.98</u>	17.65	53.35	17.55	25.52	14.52
10	<u>20.70</u>	2.10	51.62	19.01	<u>17.58</u>	<u>53.32</u>	17.50	27.05	<u>16.02</u>
null	20.35	<u>2.06</u>	51.40	18.85	17.41	53.14	17.60	<u>26.21</u>	16.35

Table 10: **Ablation study of the γ hyperparameter.** $\alpha = 0.5$ and $\beta = 0.5$ are used as default values. **Best** and **second-best** results are bolded and underlined, respectively. $\gamma \in \{2, 5, 10, \text{null}\}$.

Method	Lexical Metric			Clinical Metric					
	ROUGE-L	BLEU	BERTScore	RadGraph-F1	Temporal-F1	RaTEScore	RadEval-BERT	CheXbert _{F1} ⁵	CheXbert _{F1} ¹⁴
Baseline	19.57	<u>1.61</u>	49.56	16.23	12.11	<u>50.82</u>	<u>16.96</u>	16.14	<u>10.57</u>
+ <i>Random Setting</i>	<u>20.04</u>	1.39	<u>51.57</u>	<u>16.51</u>	<u>14.07</u>	50.29	16.85	<u>16.46</u>	10.29
+ CCD	20.70	2.10	51.62	19.01	17.58	53.32	17.50	27.05	16.02

Table 11: **Adversarial ablation study of CCD.** The *Random Setting* indicates that the signals from the expert model are replaced with randomly generated values. **Best** and **second-best** results are bolded and underlined, respectively.

This degradation in lexical metrics is attributed to the model overfocusing on symptom-related descriptions under strong probabilistic constraints. In particular, when the latent logits for certain diseases are excessively large, the model not only suppresses false positives but also amplifies existing **true positives**. As illustrated by the bar chart in Figure 2, this behaviour leads to verbose generations, which compromise the fluency and naturalness of the radiology report style. To strike a balance between clinical accuracy and lexical quality, we adopt $\beta = 0.5$ as the default setting.

Effect of γ on Guidance Strength As shown in Table 10, we evaluate the effect of varying γ , which controls the strength of the Diagnostic Plausibility Constraint in the second stage of Expert-informed Contrastive Decoding. We experiment with values of $\gamma \in \{2, 5, 10\}$ and also include a baseline where the constraint is removed entirely (denoted as null). As γ increases, the plausibility threshold becomes more relaxed, allowing the model to be more influenced by the expert model’s confidence scores. This, in turn, amplifies the suppression of false positives and the reinforcement of true positives, particularly in borderline cases. While some metrics such as RadEval-BERT and CheXbert_{F1}¹⁴ peak at lower constraint strengths, the overall performance in both lexical and clinical metrics is best balanced when $\gamma = 10$. Therefore, we adopt $\gamma = 10$ as the default setting, corresponding to a clinically meaningful threshold for severe diagnostic evidence.

F.2 Robustness Test of Clinical Contrastive Decoding with Random Prior

Since our method relies on guidance signals from a task-specific expert model, and Sec. 4.3 has demonstrated that stronger experts contribute to improved MLLM performance, it is important to assess how CCD behaves when this guidance becomes unreliable. To this end, we conduct an adversarial ablation study, where the expert model is deliberately degraded by replacing its outputs with randomly generated signals. This setting allows us to evaluate the robustness of CCD under faulty or misleading expert supervision. This experiment is conducted using MAIRA-2 (Bannur et al., 2024) as the backbone model, evaluated on the MIMIC-CXR (Johnson et al., 2019b) dataset for the radiology report generation task, with CCD hyperparameters kept at the default values.

As shown in Table 11, although the random setting introduces mild fluctuations in performance, there is no significant degradation across lexical or clinical metrics. This demonstrates that CCD does not substantially impair the MLLM’s generation quality, even when the expert signal is adversarial. These findings highlight the robustness and compatibility of our method: **it enhances downstream performance only when the expert provides meaningful guidance, while gracefully falling back to the base model’s behaviour otherwise.**

Method	Lexical Metric			Clinical Metric					
	ROUGE-L	BLEU	BERTScore	RadGraph-F1	Temporal-F1	RaTEScore	RadEval-BERT	CheXbert ⁵ _{F1}	CheXbert ¹⁴ _{F1}
Baseline	19.57	1.61	49.56	16.23	12.11	50.82	16.96	16.14	10.57
+ CCD w/ symptoms	20.70 ↑	2.10 ↑	51.62 ↑	19.01 ↑	17.58 ↑	53.32 ↑	17.50 ↑	27.05 ↑	16.02 ↑
+ CCD w/ views	20.51 ↑	1.83 ↑	51.36 ↑	17.52 ↑	14.91 ↑	52.34 ↑	16.62 ↓	10.85 ↓	7.04 ↓
+ CCD w/ devices	19.72 ↑	2.56 ↑	49.16 ↓	15.41 ↓	15.68 ↑	49.93 ↓	19.08 ↑	20.95 ↑	21.24 ↑

Table 12: **Ablation study evaluating CCD across different clinical label types.** The default label type is *symptoms*, which is replaced with *views* and *devices* to assess the sensitivity of CCD to label-type variation. “↑” indicates improvement, while “↓” denotes degradation relative to the baseline.

F.3 Evaluation of Clinical Contrastive Decoding on Additional Label Types

The proposed method relies on guidance signals from a symptom-level expert model, consistent with the design motivation of **Symptom-grounded Contrastive Decoding** described in Sec. 3.1. Sec. 4.3 further demonstrates that incorporating diverse symptom categories provides additional supervision signals that enhance MLLM performance. Therefore, it is valuable to examine whether broadening the expert concepts from symptom-level signals to include other categories, such as anatomical and observation-level findings, can still yield additional benefits. Motivated by this, the expert model types are expanded and substituted accordingly. To ensure consistency with previous analyses, the experiment follows the protocol from Sec. 4.3. The backbone is MAIRA-2 (Bannur et al., 2024), and evaluation is conducted on the MIMIC-CXR (Johnson et al., 2019b) dataset for the radiology report generation task. Default CCD hyperparameters are used throughout.

Two additional expert models are used to further assess CCD’s versatility. For the view-type expert model, the supervision signals are replaced with predictions from the binary classification models provided in TorchXRyVision (Cohen et al., 2021), covering the *Frontal* and *Lateral* radiographic views. For the device-type expert model, zero-shot classification is performed using MedSigLIP (Selbergren et al., 2025). To ensure broader coverage of common medical devices, the model considers a set of device categories adapted from prior work (Ranjit and Ganu, 2025; Sharma et al., 2025a), including: *endotracheal tube*, *tracheostomy tube*, *nasogastric tube*, *feeding tube*, *enteric tube*, *central venous catheter*, *peripherally inserted central catheter*, *chest tube*, *pigtail pleural catheter*, *pace-maker*, *implantable cardioverter-defibrillator*, and a *no-device* category.

As shown in Table 12, CCD consistently im-

proves overall performance when integrated with different expert models. Specifically, employing the *view-type* and *device-type* experts results in gains on 6 out of 9 evaluation metrics, respectively. These results highlight CCD’s ability to flexibly leverage diverse supervision signals. However, the magnitude and stability of improvement vary depending on the expert model. Notably, the symptom-type expert yields improvements across all metrics, indicating a more balanced and robust enhancement at the overall level.

G Balancing Accuracy and Ambiguity

In this section, we provide additional analysis of the two question categories that exhibited slight performance drops. As shown in Table 3, although CCD improves the overall performance of LLaVA-Med (Li et al., 2023a) on the Medical-CXR-VQA benchmark (Hu et al., 2024), two of the six evaluated categories, namely *Location* and *Type*, show a marginal decrease in accuracy. As mentioned in Sec. 4.1, we adopt a fixed set of hyperparameters across all models and tasks to ensure a fair comparison. As further discussed in Appx. E.2, we deliberately avoid tailoring hyperparameters to individual models or question types. While this promotes generality and ease of use, it may also limit performance in specific question categories that are more sensitive to decoding configurations. This trade-off reflects our focus on plug-and-play over task-specific tuning.

Figure 4 presents representative examples from the two categories with degraded performance under the default CCD hyperparameter setting. Some answers, although marked as incorrect, contain ambiguous yet clinically reasonable descriptions (highlighted in blue). While technically incorrect under strict evaluation criteria, these responses are not clearly erroneous but instead reflect overly cautious or broadly phrased interpretations, leading to borderline misjudgements.

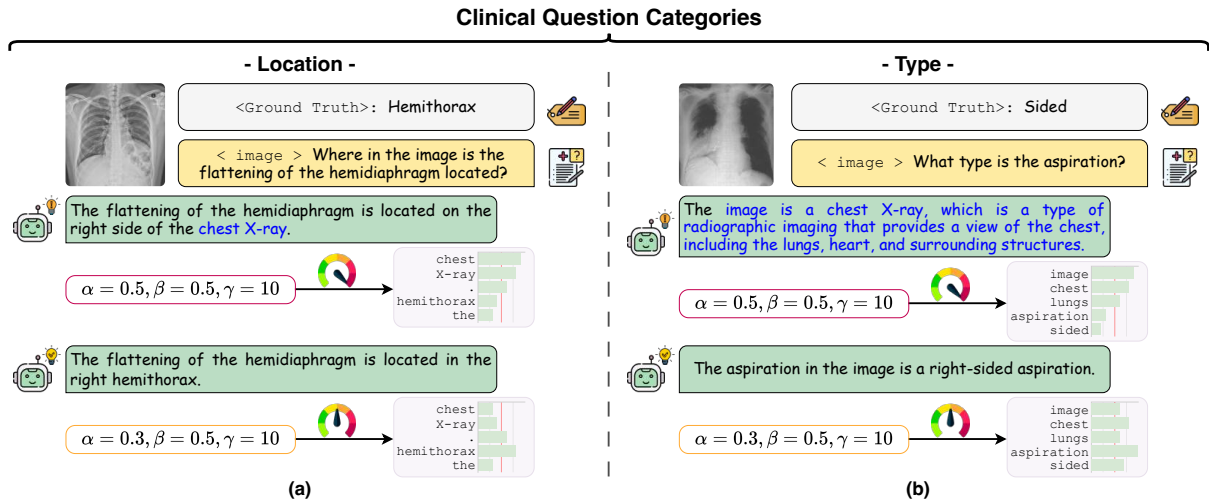


Figure 4: Illustration of additional VQA cases with CCD, using LLaVA-Med (Li et al., 2023a) as the baseline. (a) is a *location*-specific question and (b) a *type*-specific question. α , β , and λ denote CCD hyperparameters during inference. Model outputs that are vague or under-specified (i.e., partially correct but lacking clinical precision) are highlighted in blue. Latent logit ratio plots illustrate token-level differences, with (a) highlighting the final term and (b) the second token. In both cases, the top-5 overlapping tokens across two hyperparameter settings are shown as examples. The chest X-ray is blurred to preserve privacy and minimise visual discomfort.

Upon examining the latent logits distribution⁷, we observe that ground-truth tokens often have lower activation scores compared to tokens associated with more generic symptom labels. This behaviour arises from the initial anchor stage of CCD, which introduces a strong bias toward common CheXpert-related symptoms, resulting in conservative outputs. In this case, the model tends to favour frequently seen “true positive” tokens and under-represents more specific or context-dependent concepts, leading to what can be considered “dummy” false negatives.

To explore this further, we reduce the control strength of the first decoding stage by adjusting α from 0.5 to 0.3. This softens the expert guidance, allowing the model to generate more accurate and specific answers in both *Location* and *Type* categories. These findings suggest that different question types may exhibit varying levels of sensitivity to CCD’s control parameters.

While fine-grained control can improve performance for specific question categories, it also underscores a broader challenge: achieving the right balance between conservative and expressive generation. Overly cautious answers may avoid clinical errors but sacrifice specificity, while assertive responses can introduce misleading or incorrect

information. This trade-off leads to an important question in the context of medical AI: **What constitutes a “better” response in radiology MLLMs?**

“It’s better to be roughly right than precisely wrong.”

— Carveth Read

Logic: Deductive and Inductive

This quote from (Read, 1910) aptly reflects the philosophy behind our decoding strategy. In high-stakes settings such as radiology, generating responses that are somewhat ambiguous but clinically plausible is often preferable to confidently asserting inaccurate conclusions. From a system-level perspective, this approach improves overall reliability without compromising safety. CCD navigates this space by providing a balanced mechanism that moderates the influence of expert signals during generation while maintaining flexibility. Ultimately, this reflects a broader tension in aligning AI behaviour with clinical reasoning, where ambiguity, uncertainty, and contextual judgment are fundamental to the decision-making process.

H Extended Discussion on Limitations

While our study demonstrates promising results across multiple benchmarks, several limitations merit consideration, particularly in clinical applications where the requirements for safety, reliability, and interpretability are significantly more stringent than in general-purpose AI tasks.

⁷This differs from the logit plots in Figure 2, where the truncation point is defined as the token immediately following the model’s first output of a symptom phrase, namely after “Yes, the chest X-ray image shows ...”.

First, both the MIMIC-CXR (Johnson et al., 2019b) and Medical-CXR-VQA (Hu et al., 2024) datasets originate from the same institution, the Beth Israel Deaconess Medical Center. This may introduce institution-specific biases in patient demographics, imaging protocols, and clinical reporting practices, potentially limiting the generalisability of our findings to other healthcare settings with differing patient populations or workflows. Our choice of these datasets is primarily motivated by their unique status as the only publicly available sources that comprehensively align chest X-ray images with detailed free-text reports and structured question-answer annotations.

Second, all evaluations in this study rely on automatic metrics that serve only as relative references to the ground truth. While this approach is consistent with existing literature on radiology-focused MLLM evaluation, more robust validation would benefit from reader studies or expert review by licensed radiologists to further assess the clinical plausibility and safety of the generated outputs.

Third, our experiments rely on publicly available models such as MAIRA-2 (Bannur et al., 2024), of which only the 7B variant is currently open-sourced. Larger versions (e.g., MAIRA-2 13B) are not yet publicly accessible. Meanwhile, many high-performing models are only accessible via third-party APIs, which limits our ability to perform controlled experiments and to investigate scaling behaviours within our framework. This is particularly restrictive for our method, which requires direct access to the model’s latent logits space in order to apply targeted modifications. Furthermore, since our evaluations are conducted in a shared offline environment, online latency in real-world deployments may differ significantly.

Moreover, while CCD demonstrates strong performance with empirically chosen hyperparameters, it currently lacks an adaptive mechanism to adjust control strength based on task complexity, prompt context, or model uncertainty. Exploring dynamic control strategies that can respond to such internal or external signals may be a promising direction for future work—particularly for achieving a better trade-off between clinical accuracy and generation fluency across diverse applications.

In addition, most radiology MLLMs and expert models are trained on well-curated datasets like MIMIC-CXR (Johnson et al., 2019b), where image quality is standardised and acquisition conditions are controlled. As noted in Appx. B.2, these mod-

els do not cover other modalities such as computed tomography (CT), magnetic resonance imaging (MRI), or ultrasound. However, real-world clinical practice often involves lower-quality inputs, including portable X-rays or images from heterogeneous equipment. Evaluating robustness under such distribution shifts remains an important direction for future research.

In conclusion, this work takes a step toward advancing radiology-oriented multimodal language models (MLLMs) toward physician-level reasoning. Our results show that even current state-of-the-art models can be further improved by incorporating domain-specific expert models, as demonstrated by our proposed CCD framework. Although generative foundation models are developing rapidly, we believe that specialised expert models are still a necessary part of medical AI, especially in safety-critical tasks like medical imaging. This study presents a possible way to combine the strengths of both types of models to improve clinical accuracy.

I Additional Statement

In this work, we used a generative AI model to assist with colour editing and refinement of the icons in Figure 1, 2, and 4. This step was intended solely to improve visual clarity and enhance the overall readability of the figures. The use of this tool was strictly limited to visual presentation and did not influence the scientific content, analysis, or experimental results presented in the paper. We also employed Overleaf’s AI assistant to ensure spelling and grammar consistency throughout the manuscript, using UK English conventions.